

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
30 May 2003 (30.05.2003)

PCT

(10) International Publication Number
WO 03/043690 A1

(51) International Patent Classification⁷: **A61N 1/36**

Road, Allison Park, PA 15101 (US). **FIRLIK, Andrew, D.** [US/US]; 44 Still Road, Ridgefield, CT 06877 (US).

(21) International Application Number: **PCT/US02/32695**

(22) International Filing Date: 15 October 2002 (15.10.2002)

(74) Agent: **PARKER, Paul, T.**; Perkins Coie LLP, P.O. Box 1247, Seattle, WA 98111-1247 (US).

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
09/978,134 15 October 2001 (15.10.2001) US

(71) Applicant (for all designated States except US): **VERTIS NEUROSCIENCE, INC.** [US/US]; 2101 Fourth Avenue, Suite 200, Seattle, WA 98121 (US).

(81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.


(72) Inventors; and

(75) Inventors/Applicants (for US only): **GLINER, Bradford, Evan** [US/US]; 4368 230th Way SE, Sammamish, WA 98075 (US). **BALZER, Jeffrey** [US/US]; 8176 Post

(84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, SK,

[Continued on next page]

(54) Title: SYSTEMS AND METHODS FOR AUTOMATICALLY OPTIMIZING STIMULUS PARAMETERS AND ELECTRODE CONFIGURATIONS FOR NEURO-STIMULATORS

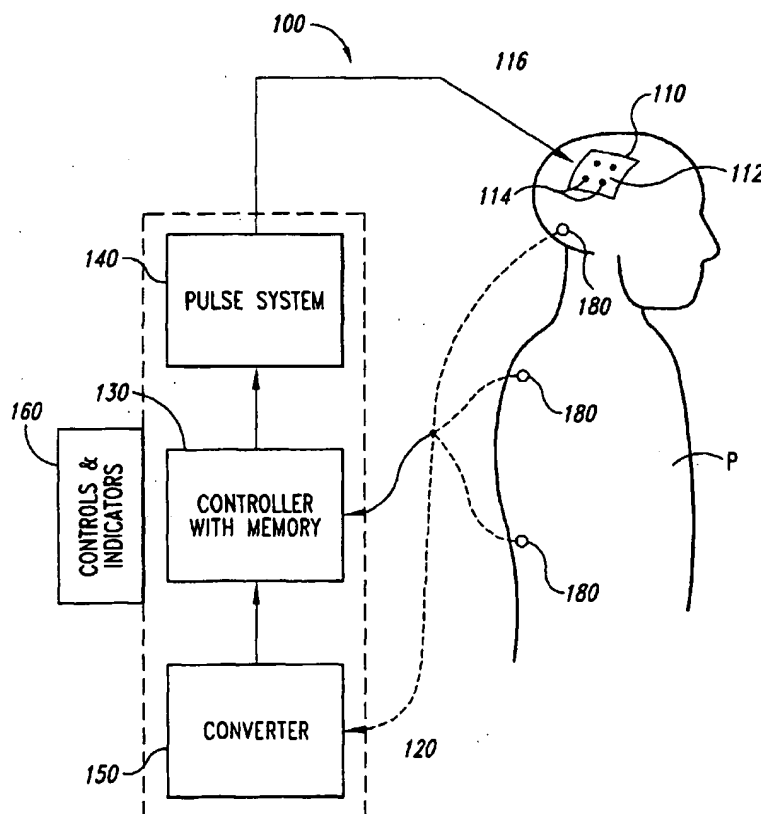

(57) Abstract: Methods and devices for automatically optimizing the stimulus parameters and/or the configuration of electrodes to provide neural stimulation to a patient. In one embodiment, a system includes an electrode array having an implantable support member configured to be implanted into a patient and a plurality of therapy electrodes carried by the support member. The system can also have a pulse system operatively coupled to the therapy electrodes to deliver a stimulus to the therapy electrodes, and a sensing device configured to be attached to a sensing location of the patient. The sensing device generates response signals in response to the stimulus. The system can also include a controller operatively coupled to the pulse system and to the sensing device. The controller includes a computer operable medium that generates command signals that define the stimulus delivered by the pulse system, evaluates the response signals from the sensing device, and determines a desired configuration for the therapy electrodes and/or a desired stimulus to be delivered to the therapy electrodes.

WO 03/043690 A1

BEST AVAILABLE COPY



TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Published:

— with international search report

SYSTEMS AND METHODS FOR AUTOMATICALLY OPTIMIZING STIMULUS PARAMETERS AND ELECTRODE CONFIGURATIONS FOR NEURO-STIMULATORS

CROSS-REFERENCE TO RELATED APPLICATION(S)

[0001] This application claims benefit of U.S. Application No. 09/978,134, filed October 15, 2001, and is a continuation-in-part of U.S. Application No. 09/802,808 filed March 8, 2001, which claims priority to U.S. Application No. 60/217,981 filed July 13, 2000, both of which are incorporated by reference herein in their entirety.

TECHNICAL FIELD

[0002] The present disclosure is related to systems and methods for automatically optimizing the configuration of therapy electrodes and/or the stimulus parameters of the electrical or magnetic waveforms applied to a target stimulation site of a patient.

BACKGROUND

[0003] A wide variety of mental and physical processes are known to be controlled or influenced by neural activity in the central and peripheral nervous systems. For example, the neural-functions in some areas of the brain (*i.e.*, the sensory or motor cortices) are organized according to physical or cognitive functions. There are also several other areas of the brain that appear to have distinct functions in most individuals. In the majority of people, for example, the areas of the occipital lobes relate to vision, the regions of the left interior frontal lobes relate to language, and the regions of the cerebral cortex appear to be consistently involved with conscious awareness, memory and intellect. The spinal cord is also organized so that specific regions of spinal cord are related to particular

functions. Because of the location-specific functional organization of the central nervous system in which neurons at discrete locations are statistically likely to control particular mental or physical functions in normal individuals, stimulating neurons at selected locations of the central nervous system can be used to effectuate cognitive and/or motor functions throughout the body.

[0004] The neural activity in the central nervous system can be influenced by electrical and/or magnetic energy that is supplied from an external source outside of the body. Various neural functions can thus be promoted or disrupted by applying an electrical current to the cortex or other part of the central nervous system. As a result, the quest for treating or augmenting neural functions in the brain, spinal cord, or other parts of the body have led to research directed toward using electricity or magnetism to control these functions.

[0005] In several existing applications, the electrical or magnetic stimulation is provided by a neural-stimulator that has a plurality of therapy electrodes and a pulse system coupled to the therapy electrodes. The therapy electrodes can be implanted into the patient at a target site for stimulating the desired neurons. For example, one existing technique for masking pain in the lower extremities of a patient is to apply an electrical stimulus to a desired target stimulation site of the spinal cord. Although determining the general location of the target stimulation site may be relatively straight forward, identifying the specific configuration of electrodes for applying the stimulus will generally vary for specific patients.

[0006] The conventional procedure for optimizing the configuration of therapy electrodes involves several steps and relies on the subjective input from the patient. Conventional techniques generally involve rendering the patient unconscious, implanting an electrode array in the patient at the stimulation site, and then letting the patient regain consciousness. After the patient is conscious, the particular configuration of electrodes is optimized for that patient by selecting different combinations of the therapy electrodes

and applying a constant electrical stimulus. The patient subjectively evaluates the effectiveness of each stimulus by indicating the degree to which the stimulus masks the pain. After testing the various configurations of therapy electrodes and deciding upon a desired electrode configuration according to the input of the patient, the patient is rendered unconscious for a second time to close the electrode array in the patient.

[0007] A similar procedure can be followed for determining the desired configuration of therapy electrodes for intra-cranial electrical stimulation. For example, a device for stimulating a region of the brain is disclosed by King in U.S. Patent No. 5,713,922. King discloses a device for cortical surface stimulation having electrodes mounted on a paddle. The paddle can be implanted under the skull of the patient so that the electrodes are on the surface of the brain in a fixed position. King also discloses that the electrical pulses are generated by a pulse generator implanted in the patient remotely from the cranium (e.g., subclavicular implantation). The pulse generator is coupled to the electrodes by a cable that extends from the paddle, around the skull, and down the neck to the subclavicular location of the pulse generator.

[0008] King discloses implanting the electrodes in contact with the surface of the cortex to create paresthesia, which is a vibrating or buzzing sensation. More specifically, King discloses inducing paresthesia in large areas by placing the electrodes against particular regions of the brain and applying an electrical stimulus to the electrodes. This is similar to implanting therapy electrodes at the spinal cord of a patient for masking pain in the lower extremities of a patient, and thus King appears to require stimulation that exceeds the membrane activation threshold for a population of neurons at the electrodes (supra-threshold stimulation). King further discloses applying a stimulus to one set of electrodes, and then applying a stimulus to a separate configuration of electrodes to shift the location of the paresthesia.

[0009] One problem of the procedures for optimizing the configuration of therapy electrodes for either spinal or cortical stimulation is that existing

systems and methods are expensive and time consuming. First, it is expensive to render the patient unconscious, implant the neural-stimulators in the patient, then wait for the patient to regain consciousness, then test various electrode configurations by asking the patient to subjectively estimate the degree to which the particular stimulus masks the pain, and then finally render the patient unconscious again to complete the implantation. Second, it can be a reasonably high risk operation because the patient is placed under general anesthesia at two separate stages of the process. It will be appreciated that this is an extremely long process that requires highly skilled doctors and personnel to attend to the patient for a significant period of time. Moreover, the patient occupies costly operating rooms and utilizes expensive equipment throughout the process. Third, relying on the subjective response from the patient may not provide accurate data for evaluating minor variances in the results. Fourth, the patient may experience pain or discomfort because some configurations may provide high intensity stimulation that exceeds the sensory level of stimulation. Therefore, existing systems for determining a desired configuration of electrodes to apply a neural-stimulus to specific patients are expensive, time consuming, potentially painful, and may not determine the most effective electrode configuration.

[0010] Another drawback of configuring the therapy electrodes using existing systems and methods is that the procedures are not effective for on-going use. This is because the patient's condition changes continually. For example, the location of the pain or the sensation typically shifts over time such that the optimal configuration of the electrodes at one point of the therapy may not mask the pain after a period of time. A large number of patients accordingly terminate electrical therapies for paresthesia within one year because of such a shift in the location of the pain/sensation. Therefore, although electrical stimulation for masking pain, inducing or enhancing plasticity, and other reasons appears to be very promising, it has not yet gained wide acceptance because of the drawbacks of configuring the

therapy electrodes to apply an effective stimulus to different patients over a long period of time.

[0011] Additionally, it is also difficult to optimize the parameters of the electrical or magnetic stimulus. For example, even when a desired configuration of therapy electrodes is used, different waveforms can produce different results in each patient. Determining the stimulus parameters of the waveform can be even more time consuming than determining the desirable configuration of therapy electrodes because it involves testing a large number of independent variables. In a biphasic pulse train, for example, the stimulus parameters can include (a) the intensity of the electrical current, (b) the time of the stimulus of the first phase, (c) the time of the stimulus of the second phase, (d) the total time of the stimulus pulse, (e) the frequency of the stimulus pulse, (f) the pulse duty cycle, (g) the burst time of the stimulus, (h) the burst repetition rate of the stimulus, and (i) additional variables. Because of the large number of stimulus parameters, a particular waveform for the stimulus is typically selected for a given treatment for all patients such that the parameters for stimulus itself are not optimized.

[0012] In light of the several drawbacks for existing techniques of applying electrical or magnetic neural-stimulation to produce desired results, there is a significant need to enhance the procedures for applying such stimulus to individual patients. For example, it would be desirable to have more cost effective and less time consuming procedures for determining an effective configuration of therapy electrodes and stimulus parameters. Additionally, it would be desirable to update the electrode configuration and stimulus parameters in each individual patient without surgically operating on the patient to compensate for shifts in the target stimulation site.

BRIEF DESCRIPTION OF THE DRAWINGS

[0013] Figure 1 is a schematic illustration of a system for automatically optimizing the configuration of the electrodes and/or the stimulus parameters in accordance with an embodiment of the invention.

- [0014] Figure 2 is a flow diagram illustrating a method for automatically optimizing the configuration of electrodes and/or the stimulus parameters in accordance with one embodiment of the invention.
- [0015] Figure 3 is a flow diagram of an embodiment of a method for optimizing the configuration of therapy electrodes that can be used in the method of Figure 2 in accordance with an embodiment of the invention.
- [0016] Figures 4A-4F illustrate various examples of using the system of Figure 1 to optimize the configuration of the electrodes in accordance with an embodiment of the methods of Figures 2 and 3.
- [0017] Figure 5 is a flow diagram of a method for optimizing the stimulus parameters that can be used in the method of Figure 2 in accordance with an embodiment of the invention.
- [0018] Figure 6 is a diagram illustrating an example of several stimulus parameters that can be optimized using an embodiment of the method of Figure 5.
- [0019] Figure 7 is a flow diagram of a method for optimizing the electrode configuration and/or stimulus parameters for inducing and/or enhancing neural-plasticity using sub-threshold stimulation in accordance with an embodiment of the invention.

DETAILED DESCRIPTION

- [0020] The following disclosure describes several methods and apparatus for automatically determining the configuration of therapy electrodes and/or the parameters for the stimulus to treat or otherwise effectuate a change in neural-functions of a patient. Several embodiments of methods in accordance with the invention are practiced using a computer to automatically implement such processes, but it is not necessary to use a computer in all of the embodiments. The specific details of certain embodiments of the invention are set forth in the following description and in Figures 1-7 to provide a thorough understanding of these embodiments to a person of ordinary skill in the art. More specifically, several embodiments of

a system in accordance with the invention are described with reference to Figure 1, and then several embodiments of methods for determining a desired configuration of therapy electrodes and/or stimulus parameters are described with reference to Figures 2-7. A person skilled in the art will understand that the present invention may have additional embodiments, or that the invention can be practiced without several of the details described below.

A. SYSTEMS FOR AUTOMATICALLY OPTIMIZING THERAPY
ELECTRODE CONFIGURATIONS AND/OR STIMULUS
PARAMETERS

[0021] Figure 1 illustrates an embodiment of a system for providing neuro-stimulation to a patient that can automatically optimize (a) the configuration of therapy electrodes, (b) the waveform parameters for the electrical stimulus, and/or (c) additional stimulation parameters. In this embodiment, the system 100 comprises an electrode array 110, a stimulus unit 120 operatively coupled to the electrode array 110, and at least one sensing device 180 operatively coupled to the stimulus unit 120. The electrode array 110 and the sensing unit 180 can be operatively coupled to the stimulus unit 120 by a direct connection (e.g., wires, cables, or fiber optical lines) or an indirect connection (e.g., RF energy, magnetic energy, infrared, etc.).

[0022] The electrode array 110 can include a support member 112 and a plurality of electrodes 114 that are carried by the support member 112. The electrode array 110 is generally configured to be implanted into a patient *P* for cortical stimulation, deep brain stimulation, spinal cord stimulation, cardiac stimulation, or stimulation of other parts of the body. For example, the electrode array 110 can be a cortical neural-stimulation device, such as one of the devices described in U.S. Application No. 09/802,808 incorporated by reference above. The electrode array 110 can alternatively be a grid having a plurality of discrete electrodes 114 arranged in an X-Y coordinate system or another type of coordinate system. The therapy

electrodes 114 can be independently coupled to the stimulus unit 120 by a link 116. In one embodiment, the link 116 is a wire or another type of conductive line, but in alternate embodiments the link 116 can be an indirect link (e.g., infrared, magnetic or RF energy). The link 116 can accordingly be a direct connection or an indirect connection to operatively couple the therapy electrodes 114 to the stimulus unit 120. It will be appreciated that many of the electrode arrays can be implanted at the spinal cord for spinal cord stimulation.

[0023] The stimulus unit 120 can include a controller 130 with a processor, a memory, and a programmable computer medium. The controller 130, for example, can be a computer and the programmable computer medium can be software loaded into the memory of the computer and/or hardware that performs the processes described below. The stimulus unit 120 can further include a pulse system 140, a converter 150, and a plurality of controls/indicators 160. The pulse system 140 can generate and send energy pulses to the electrode array, and the converter 150 can receive signals from the sensing device 180. The pulse system 140 and the converter 150 are both operatively coupled to the controller 130. The controls and indicators 160 can include a computer display, an input/output device (e.g., a keyboard, touch sensitive screen, etc.), or other types of devices commonly used to enter commands or receive output from computers.

[0024] The electrode array 110 and the pulse system 140 can be integrated into a single stimulation apparatus that can be implanted into the patient, as described in U.S. Application No. 09/082,808. One example of an integrated pulse system 140 and electrode array 110 is configured to be implanted into the skull of the patient so that the electrodes contact the pia matter of the cortex. Such a device can have an internal power source that can be implanted into the patient and/or an external power source coupled to the pulse system via electromagnetic coupling or a direct connection. In alternate embodiments, the pulse system 140 is an external unit that is not

implanted into the patient. The external pulse unit 140 can provide the electrical stimulus to the therapy electrodes 114 using RF energy, electromagnetism, or wire terminals exposed on the scalp of the patient *P*.

[0025] The sensing device 180 can be an electrode that produces an analog signal, and the converter 150 can convert the analog signal to a digital signal for processing by the controller 130. The sensing device 180 can be an implantable electrode that can be implanted at a number of different locations according to the desired response of the stimulus applied to the therapy electrodes 114. In alternate embodiments, the sensing device 180 can be an imaging device (e.g., an fMRI apparatus), an ultrasound apparatus, an EEG, a device that detects somatosensory evoked potentials, or another suitable apparatus for determining a response in the patient *P* to a stimulus applied to the therapy electrodes 114. The sensing device can alternatively detect behavioral responses. In an alternate embodiment, the sensing device 180 can produce a digital output and be coupled directly to the controller 130. Therefore, the converter 150 may only be used in some of the embodiments of the system 100.

[0026] The system 100 can automatically test the efficacy of various electrode configurations and stimulus parameters either with or without subjective input from the patient. In operation, the controller 130 sends command signals to the pulse system 140 defining the configuration of active electrodes and the waveform parameters for the stimulus. The pulse system 140 generates and sends a single pulse or pulse train to the active therapy electrodes in accordance with the command signals, and the sensing device 180 senses the neural responses, motor responses, or other types of responses to the stimulus. The sensing device 180 also sends signals corresponding to the magnitude of the responses to the controller 130, which compares the responses to previous responses and/or empirical responses for the type of therapy stored in the memory of the controller. The controller 130 then adjusts the configuration of active therapy electrodes and/or the waveform parameters of the stimulus to optimize the

therapy for the particular patient. Several methods for using embodiments of the system 100 for supra- and sub-threshold neural-stimulation therapies are described below.

B. METHODS OF OPTIMIZING ELECTRODE CONFIGURATIONS AND STIMULUS PARAMETERS FOR NEURO-STIMULATION

[0027] Figures 2-7 illustrate several embodiments of methods in accordance with the invention that can be practiced using the stimulator system 100 described above. Figure 2, for example, is a flow diagram illustrating an optimization process 200 that can be executed, at least in part, in a computer for automatically optimizing the configuration of therapy electrodes and/or the waveform parameters for the stimulus. The optimization process 200 generally starts after the therapy electrode array has been installed at a target stimulation site using surgical techniques known in the art and a sensing device has been positioned to sense a response to the electrical stimulus applied to the therapy electrodes.

[0028] After the therapy electrode array has been installed and the sensing device is ready to sense a response in the patient, the optimization process 200 begins with a setup procedure 210 in which a setup configuration of therapy electrodes and the waveform parameters for a control stimulus are selected. The controller can select the setup configuration for the electrodes and the control stimulus by retrieving predetermined setup values stored in a setup database in the memory of the controller. The setup database can contain at least one setup configuration for the therapy electrodes and at least one set of waveform parameters for the control stimulus. In several embodiments, a plurality of different setup configurations for the electrodes and the stimulus parameters can be stored in a database so that the system 100 can be used for many different types of neural therapies and procedures. An alternate embodiment can involve manually inputting the setup configuration for the electrodes and the waveform parameters for the control stimulus either in lieu of or in addition to having the controller retrieve

setup data from memory. A practitioner, for example, can select the setup data from pull-down menus provided by the system 100 or manually key in the data.

[0029] The setup configurations for the therapy electrodes and the waveform parameters for control stimuli can be determined by manually performing optimization procedures on test groups of patients for each type of therapy. The optimal setups can be correlated with the particular therapy (e.g., enhancing neural plasticity in the cortex, masking pain, etc.), the particular target site, and the patient factors. For example, a first electrode configuration and control stimulus can be determined for sub-threshold cortical neural stimulation to restore functionality of a limb that was affected by a stroke or other type of brain damage; a second electrode configuration and control stimulus can be determined for cortical neural stimulation to enhance learning capabilities; a third electrode configuration and control stimulus can be determined for spinal stimulation to mask pain; and a fourth electrode configuration and control stimulus can be determined for sub- or supra-threshold stimulation applied to the cortex. It will be appreciated that many additional electrode configurations and stimulus parameters can be determined for other types of therapies such that the foregoing is not exhaustive of the various types of setup configurations.

[0030] Referring again to Figure 2, the optimization process 200 continues with a stimulating procedure 220 and then a sensing procedure 230. The stimulating procedure 220 involves applying an electrical stimulus to a configuration of the therapy electrodes. Several iterations of the stimulation procedure 220 are generally performed several times at different stages throughout the optimization process 200, and the configuration of the electrodes and/or the stimulus parameters can be changed at each iteration of the stimulation procedure 220. For example, the initial iteration of the stimulating procedure 220 can involve applying the control stimulus to the setup configuration of therapy electrodes. Subsequent iterations of the stimulation procedure 220 can involve applying (a) the control stimulus to an

alternate configuration of therapy electrodes; (b) an alternate stimulus with a different waveform to the setup electrode configuration; and/or (c) alternate stimuli with different waveforms to alternate electrode configurations. As explained above with reference to Figure 1, the controller carries out the stimulation procedure 220 by sending command signals to the pulse system, which in turn generates and transmits energy having the parameters for the stimulus to the selected configuration of active therapy electrodes.

[0031] The sensing procedure 230 is generally performed after each iteration of the stimulation procedure 220. The sensing procedure 230 involves monitoring a location in the patient for a response to the stimulus applied in the stimulation procedure 220. The location for sensing the response and the particular type of response that is measured varies according to the particular type of therapy and other factors. In general, the physiologic outcome that the response measures can be categorized into three general areas: (1) cortical; (2) peripheral; and (3) functional. The types of measurements for monitoring cortical physiologic outcomes include: (a) action potential generation of the neurons; (b) excitability changes of the neurons measured waveform characteristics of EEG or field potentials within the cortex; (c) blood flow (e.g., doppler measurements); (d) thermal changes; (e) pulse oxymetry; (f) chemical metabolites; and (g) imaging techniques (e.g., functional MRI, MR spectroscopy, diffusion MRI, PET, CT, etc.). The types of measurements for monitoring peripheral physiologic outcomes include: (a) EMG (surface, percutaneous, or implanted); (b) external potentiometer or other forms of physiologic input; and (c) motion detectors (e.g., accelerometers). The types of measurements for monitoring functional physiologic outcomes include: (a) force/strength tests; (b) dexterity tests; (c) speed/reflex tests; and (d) performing complex tasks.

[0032] Several types of measurements that monitor the physiologic outcomes can be automated so that they generate signals which can be processed by the controller either with or without subjective input from the patient. In the case of EMG measurements for sensing peripheral

responses to the applied stimulus, the electrical signals from the EMG sensors are automatically received and processed by the controller. In other applications, the data sensed by functional MRI, blood flow monitors, thermal monitors, pulse oxymeters, PET, MR spectroscopy, accelerometers, etc. can be digitized and process by the controller in a similar manner. In this manner, the stimulating procedure 220 and the sensing procedure 230 can be automated using a controller with the appropriate hardware and/or software.

[0033] The optimization process 200 also includes performing an evaluation procedure 240 after one or more iterations of the stimulating procedure 220 and the sensing procedure 230. The evaluation procedure 240 can involve a determination routine 242 in which a sensed response from the sensing procedure 230 is compared with a desired response range and/or other responses from previous iterations of the stimulation procedure 220 and the sensing procedure 230. Based upon whether the sensed response is within a desired range and/or shows an improvement compared to previous responses or target ranges, the controller can automatically test the effectiveness of other electrode configurations and stimulus parameters. For example, if the response is not within the desired response range, then the determination routine 242 directs the controller to select an alternate configuration for the therapy electrodes and/or alternate parameter for the stimulus. Alternatively, in one embodiment when the sensed response is within the desired response range, the determination routine 242 can direct the controller to proceed directly to a stop 270 and indicate that the configuration of therapy electrodes and the parameters for the stimulus have been optimized to treat the specific patient. In another embodiment when the sensed response is within the desired response range, the determination routine 242 directs the controller to select additional alternate configurations of the therapy electrodes and/or stimulus parameters to discover whether a more effective response can be achieved.

[0034]

The process of selecting alternate therapy electrode configurations or stimulus parameters is performed by an analyzing procedure 260. In one embodiment, the analyzing procedure 260 is predicated upon the understanding that the electrode configuration and each of the stimulus parameters are independent variables that can be individually optimized while keeping the other variables constant. The analyzing procedure 260, therefore, can proceed by keeping one of the configuration of the therapy electrodes or the stimulus parameters constant and then progressively adjusting the other of these variables until the most effective result is obtained for the adjusted variable. For example, when the analyzing procedure 260 selects alternate stimulus parameters, it typically maintains the previous configuration of therapy electrodes and it adjusts only one of the stimulus parameters at a time. Conversely, the analyzing procedure 260 can keep the same stimulus parameters and select alternate configurations of therapy electrodes. The analyzing procedure 260 can select alternate inputs for the stimulus parameters and/or the electrode configurations by dynamically estimating new parameters based on projected response patterns for using empirical data developed for particular therapies and/or actual responses from previous stimuli applied to the patient. In one embodiment, the controller automatically analyzes the responses from previous stimulating procedures 220 to determine a pattern of improved or degraded effectiveness of the corresponding configurations of therapy electrodes and stimulus parameters that were applied in the iterations of the stimulation procedure 220. Based upon the pattern of responses, the analyzing routine 260 can then incrementally change one of the variables in a manner that concurs with a pattern showing improved responses or moves away from the pattern that shows deteriorated responses.

[0035]

A basic example of the analyzing routine 260 involves optimizing the frequency of the electrical stimulus. As such, the configuration of electrodes and the other stimulus parameters remain constant for several iterations of the applying procedure 220. In one iteration a stimulus having a first

frequency (e.g., 50 Hz) may produce marginal results as determined by the sensing and evaluation procedures 230 and 240. Without additional data, the analyzing procedure 260 selects a second stimulus with a second frequency either less or greater than the first frequency to get a general understanding of whether higher or lower frequencies produce more efficacious results. The controller, for example, can select a second frequency of 25 Hz. If a frequency of 25 Hz produces better results than 50 Hz, the controller can select still lower frequencies in the analyzing procedure 260; but, assuming for the sake of this example that a frequency of 25 Hz produces a worse result than 50 Hz, then the controller can select a third frequency higher than the second frequency (e.g., 100 Hz). If the higher third frequency (e.g., 100 Hz) produces a better result than the first frequency (e.g., 50 Hz), then the controller can select a still higher fourth frequency (e.g., 200 Hz) in a subsequent iteration of the procedure. The method 200 can continue in this manner by adjusting variables in a direction that produces better results until the results begin to deteriorate. At this point, it is expected that the optimal value for the variable is bracketed between the last value selected for the variable and the value of the iteration immediately preceding the penultimate iteration (i.e., the second-to-the-last iteration).

[0036] Several embodiments of the optimization procedure 200 that use the system 100 are expected to reduce the cost and time for optimizing the configuration of the therapy electrodes and the stimulus parameters. One feature of the optimizing method 200 is that the pulse system and the therapy electrodes can be an integrated unit that is implanted into the patient and controlled externally from the patient such that an external controller can adjust the variables (e.g., electrode configuration and/or stimulus parameters) without requiring opening the patient for access to the pulse system and/or the therapy electrodes. One benefit of this feature is that several different electrode configurations and stimulus parameters can be adjusted after implanting the electrode array, and the variables can also

be tested rather quickly because the controller can automatically adjust the variables and apply the stimulus to the therapy electrodes in a manner that is expected to be much faster than manually adjusting the variables. Another benefit of this feature is that the patient need only be subject to a single application of an anesthetic because the patient can be closed up soon after implanting the electrode array and the test can be performed after closing the patient. As a result, several embodiments of the optimization procedure 200 are expected to reduce the time and costs for determining a desirable electrode configuration and stimulus parameters.

[0037] Several embodiments of the optimization procedure 200 are also expected to provide better results than relying solely on the subjective input of the patient. Another aspect of several embodiments of the system 100 is that the sensing device provides objective criteria that measures the response to the stimuli. This feature is expected to provide better accuracy in determining the effectiveness of the individual stimuli applied to the therapy electrodes. Moreover, the optimization procedure 200 can also expediently optimize the waveform parameters in addition to optimizing the configuration of therapy electrodes such that both the electrical components of the stimulus and the location(s) where the stimulus is applied are optimized for specific patients.

[0038] Another feature of several embodiments of the optimization method 200 using the system 100 is that they are expected to provide more effective therapies over a long period of time without additional surgical procedures. One feature that provides this benefit is that the pulse system and the electrode array can be implanted into the patient and controlled externally from the patient. As a result, when the effectiveness of the therapy degrades because the target site shifts or another variable changes, the sensing device 180 can be positioned relative to the patient and coupled to the controller to re-optimize the electrode configuration and/or the stimulus parameters without having to perform surgery on the patient. The system 100 can accordingly be operated using embodiments of the optimization

procedure 200 at any time to compensate for shifts in the target location. Several embodiments of the optimization procedure 200 that use the system 100 are accordingly expected to provide more effective therapies for ongoing applications.

[0039] Still another benefit of several embodiments of the method 200 is that they are expected to be more comfortable for patients. One feature of the method 200 is that the sensing procedure can sense responses at levels that the patient cannot feel any sensations. As a result, is it not likely that the application of the stimulus will cause pain or discomfort.

[0040] Figure 3 is a flow diagram illustrating one embodiment of a method for optimizing the configuration of therapy electrodes in accordance with the invention. In this embodiment, the method 300 can include a setup procedure 310 in which a setup configuration of therapy electrodes is selected. The setup configuration of therapy electrodes can be based upon historical data obtained from previous optimization procedures for specific patients or different types of therapies. After performing the setup procedure 310, the method 300 continues with a stimulating procedure 320 in which a control electrical stimulus is applied to the selected configuration of therapy electrodes. A response in the patient to the applied control stimulus is then sensed in a sensing procedure 330, which is generally performed after each iteration of the stimulating procedure 320. The stimulating procedure 320 and the sensing procedure 330 can be similar to those described above with reference to Figure 2, except that the stimulating procedure 320 involves applying the same control stimulus for each iteration. The primary difference, therefore, is that the configuration of therapy electrodes can be changed for each iteration of the stimulating procedure 320.

[0041] The method 300 continues with an evaluation procedure 340 in which the sensed response from the sensing procedure 330 is compared with a predetermined range of desired responses and/or previous responses from the sensing procedure 330. The evaluation procedure 340 can have several

different embodiments. The evaluation procedure 340, for example, can include a determination routine 342 that determines whether the sensed response is the optimized response. In one embodiment, the sense response is considered to be optimized when it is within a desired range of responses. The method 300 can accordingly proceed to stop when such a response is sensed. In another embodiment, the sensed response is considered to be optimized when it provides the best result of all possible configurations of electrodes. This embodiment generally involves applying the control stimulus to all possible configurations of electrodes before identifying the optimized electrode configuration. In still another embodiment, the sensed response is the optimized response when it provides the most effective result compared to other responses without testing all of the possible configurations of electrodes. This embodiment involves testing a number of electrode configurations, identifying a trend in electrode configurations that produce effective results, and determining if or when the trend no longer holds true. It will be appreciated that the evaluation procedure 340 can have several additional or different embodiments.

[0042] The method 300 can continue with an analyzing procedure 360 that selects an alternate therapy electrode configuration. The alternate therapy electrode configuration selected in the analyzing procedure 360 can be determined by comparing previous responses to other configurations of therapy electrodes to develop a pattern of improved responses and selecting a configuration that is expected to continue the trend. Alternatively, the analyzing procedure 360 can simply select another therapy electrode configuration that has not yet been tested. The method can also include a final selection procedure 365 that selects the optimized configuration of the therapy electrodes based upon the sensed responses. The process 300 can then terminate with a final stop procedure 370 in which the optimized electrode configuration is stored in memory, displayed to a practitioner, or otherwise presented for use.

[0043] Figures 4A-4L illustrate several examples of therapy electrode configurations that can be selected in the analyzing procedure 360 and then tested in the stimulating procedure 320, the sensing procedure 330, and the evaluation procedure 340. In these embodiments, a therapy electrode array 400 for use with the system 100 (Figure 1) can include an implantable support member 410 and a plurality of electrodes 420 carried by the support member 410. The therapy electrodes 420 can be individual electrodes that are arranged in a grid array having M columns and N rows. The electrode array 400 can have several other arrangements of electrodes 420, such as concentric circles, elongated lines, or many other patterns. Each of the electrodes 420 can be independently coupled to a pulse system so that individual electrodes 420 can be activated or inactivated using the controller 130 (Figure 1) and the pulse system 140 (Figure 1). The electrode array 400 is typically implanted into the patient so that the electrodes 420 are placed generally over or proximate to a target location T for stimulation. In many embodiments, the target location T can be at the surface of the cortex, along the spinal cord, or within a deep brain region of a patient depending upon the particular treatment being applied to the patient.

[0044] Figures 4A and 4B illustrate two alternate embodiments of selecting therapy electrode configurations. Referring to Figure 4A, a setup configuration of two active electrodes 420a can be selected such that the electrodes are within the target location T . One of the active electrodes 420a can be biased with a positive polarity and the other active electrode 420a can be biased with a negative polarity. Referring to Figure 4B, a subsequent iteration of the process can include selecting an alternate configuration of therapy electrodes in which the polarity of the active electrodes 420a is switched. Figures 4C-4E illustrate alternate embodiments of selecting different configurations of therapy electrodes using the analyzing procedure 360 explained above with reference to Figure 3. As can be seen from Figures 4C-4E, the active therapy electrodes 420a can be inside and/or outside of the target location T . Figure 4C illustrates an

embodiment in which all of the active electrodes 420a are within the target location and adjacent to one another, and Figures 4D and 4E illustrate embodiments in which at least some of the active electrodes 420a are outside of the target location T and one or more inactive electrodes 420 are between some of the active electrodes 420a. It will be appreciated that the analyzing procedure 360 can select any configuration of therapy electrodes 420 in the $M \times N$ electrode array 400 such that any combination of electrodes 420 can be active electrodes.

[0045] Figure 4F illustrates another aspect of selecting a desired configuration of therapy electrodes in which an original target location T_o (shown in broken lines) has changed to a current target location T_c . The shift from the original target location T_o to the current target location T_c can be caused by several generally unpredictable factors. The methods 200 and 300 can compensate for such a target location shift without additional surgery because the therapy electrodes can be optimized using an external control and indirect coupling with the pulse system and/or or the electrode array. Thus, the application of the stimulus can be changed as the target location of neural activity shifts to provide efficacious treatment over a long period of time.

[0046] Figures 4G and 4H illustrate different embodiments of therapy electrical configurations that can be selected in the analyzing procedure 360 in which several electrodes on opposite areas of the target location are activated with a common polarity. Referring to Figure 4G, for example, this embodiment illustrates a series of active electrodes on opposite ends of the target location T . One embodiment of this configuration applies a common polarity to a first set 420_{a1} of active electrodes and an opposite polarity to a second set 420_{a2} of active electrodes. Another embodiment can apply the same polarity to all of the active electrodes in both of the sets 420_{a1} and 420_{a2}. Figure 4H illustrates a related embodiment in which a number of electrodes on opposite sides of the target location T are active electrodes. The electrode configuration shown in Figure 4H can also apply a common

polarity to all of the active electrodes on each side of the target location T or all of the electrodes on both sides of the target location T .

[0047] Figures 4I and 4J illustrate additional embodiments of electrode configurations that can be selected in the analyzing procedure 360 and then tested in the stimulation procedure 320. Figure 4I illustrates an embodiment in which a first set 420_{a1} of active electrodes has a common polarity at one end of the target location T , and a second set 420_{a2} of active electrodes is located at an opposite end of the target location T . The polarity of the electrodes in the second set 420_{a2} can be opposite or the same as those of the active electrodes in the first subset 420_{a1} . Figure 4J illustrates a similar embodiment in which a first set 420_{a1} of active electrodes is located within the target location T along one side, and a second set 420_{a2} of active electrodes is located within a target location T along an opposite side. The electrodes in the first set 420_{a1} can have one polarity, and the electrodes in the second set 420_{a2} can have an opposite polarity.

[0048] Figures 4K and 4L illustrate additional embodiments of therapy electrode configurations that can be selected in the analyzing procedure 360 and then tested in the stimulation procedure 320. Referring to Figure 4K, this embodiment illustrates a first set 420_{a1} of active electrodes at one end of the target location T and a second set 420_{a2} of active electrodes at an opposite end of the target location T . The active electrodes in the first set 420_{a1} can have opposite polarities and similarly the active electrodes in the second set 420_{a2} can have opposite polarities. The active electrodes in the first and second sets 420_{a1} and 420_{a2} can be located outside of the target location T as shown in Figure 4K. Figure 4L illustrates a related embodiment in which the active electrodes in the first set 420_{a1} have opposite polarities, and the active electrodes in the second set 420_{a2} have opposite polarities. The active electrodes in the first and second sets 420_{a1} and 420_{a2} shown in Figure 4L are located within the boundaries of the target location T . It will be appreciated that the invention can have several additional embodiments in which the individual sets of electrodes can be

inside, outside, inside and outside, and have different combinations of polarities.

[0049] Another aspect of the invention is optimizing the parameters for the electrical stimulus in addition to or in lieu of optimizing the configuration of therapy electrodes. Figure 5 is a flow diagram of a method for optimizing the desired parameters for the electrical stimulus in accordance with an embodiment of the invention. In this embodiment, the method 500 can include a setup procedure 510 in which a therapy electrode configuration and the initial parameters for the electrical stimulus are selected. The configuration of therapy electrodes can be the optimized configuration from the method 300 explained above with reference to Figure 3, or it can be another configuration input by a practitioner or retrieved from memory in the controller. The same configuration of therapy electrodes is generally maintained throughout the method 500. After performing the setup procedure 510, the method 500 continues with a first stimulating procedure 520 in which the electrical stimulus is applied to the selected configuration of therapy electrodes using the initial parameters of the electrical stimulus. A response in the patient to the initial electrical stimulus is sensed in a first sensing procedure 530. The procedures 510-530 accordingly provide a response to an initial electrical stimulus based upon the initial stimulus parameters to provide a baseline response.

[0050] The method 500 continues with an adjusting procedure 540 in which one of the stimulus parameters for the electrical stimulus is adjusted, and then a second stimulating procedure 550 in which the adjusted stimulus is applied to the therapy electrodes. A response to the adjusted stimulus is then determined using a second sensing procedure 560. The method 500 can repeat the procedures 540-560 several times for each of the parameters of the electrical stimulus to develop a plurality of responses for each parameter.

[0051] The method 500 can then continue with an evaluation procedure 570 in which the responses are evaluated to determine specific values for the

stimulus parameters that provide an efficacious result. The evaluation procedure 570 can include a determination routine 572 that determines whether a parameter of the stimulus has been optimized. If the response for a parameter is not optimized, then the method can continue by repeating the procedures 540-560 for the parameters that are not within a desired range. However, if the response is optimized, then the determination routine 572 can continue to a final selection procedure 580 in which a set of electrical parameters that produce a desirable response are selected.

[0052] Figure 6 is a graph illustrating some of the stimulus parameters that can be optimized using the method 500. A stimulus start time t_0 defines the initial point at which an electrical or magnetic pulse is applied to the therapy electrodes. For a biphasic waveform, the parameters typically include a pulse width t_1 for a first phase, a pulse width t_2 for a second phase, and a stimulus pulse width t_3 for a single biphasic pulse. The pulse can alternatively be a monophasic pulse. The parameters can also include a stimulus repetition rate $1/t_4$ corresponding to the frequency of the pulses, a stimulus pulse duty cycle equal to t_3 divided by t_4 , a stimulus burst time t_5 that defines the number of pulses in a pulse train, and/or a stimulus pulse repetition rate $1/t_6$ that defines the stimulus burst frequency. Another parameter of the electrical stimulus is the intensity of the current I_1 for the first phase and the current intensity I_2 for the second phase of each pulse. In another embodiment, a continuous pulse train can be used such that $t_5=t_6$.

[0053] In a typical application, one of the parameters is adjusted for each application of the stimulus while maintaining the other parameters constant to determine the affect that adjusting the one parameter has on the response in the patient. Each of the parameters are believed to be independent from one another, thus one of the parameters can be optimized by applying a number of different stimuli using different values for the parameter to determine whether increasing or decreasing the parameter enhances the efficacy of the stimulus. Once it is determined whether increasing or decreasing the parameter provides a better result, then the

parameter can be further increased or decreased (whichever is more desirable) until the effectiveness of the stimulation degrades. The optimized value for a particular stimulus parameter can then be stored in memory, and then a different stimulus parameter can be optimized using a similar procedure for that parameter. As such, one or more of the stimulus parameters can be optimized using this procedure.

[0054] The embodiments of the methods 200, 300 and 500 described above can be used to optimize procedures for cortical stimulation, spinal stimulation, deep brain stimulation, and peripheral stimulation for a number of different applications. The spinal stimulation and certain aspects of the cortical stimulation can be used to mask pain, such as back pain, phantom limb pain experienced by amputees, or pain in the lower extremities. The deep brain stimulation can be optimized to treat movement disorders (e.g., Parkinson's disease, dystonia, etc.), depression, or other functions related to deep brain neural activity. The methods can also be used to optimize therapies for cortical stimulation that enhance learning functions, restore motor functions (e.g., use of muscle groups affected by stroke or other trauma), and treating diseases or seizures (e.g., Alzheimer's, epilepsy, etc.). Many of the embodiments of the methods 200, 300 and 500 for masking pain involve applying supra-threshold activation stimuli to the therapy electrodes. On the other hand, several of the cortical neural-stimulation procedures that are not directed toward masking pain but rather seek to enhance existing functions (e.g., learning) or rehabilitate impaired functions (e.g., brain damage) use sub-threshold activation stimuli that do not exceed the membrane activation threshold of a population of neurons in the target stimulation site. Several embodiments of the methods 200, 300 and 500 that are directed more specifically toward sub-threshold optimization of the neural-stimulation procedures are described below with reference to Figure 7.

C. SUB-THRESHOLD OPTIMIZATION METHODS

[0055] Figure 7 is a flow diagram illustrating an embodiment for optimizing a sub-threshold simulation therapy. Sub-threshold simulation involves training and/or recruiting neurons to perform a neural-function. The target location can be a site where neural-plasticity is occurring or is expected to occur. The present inventors believe that neurons become more likely to be able to carry out desired neural-functions for enhancing, repairing or restoring functionality after being stimulated electrically at a level below the membrane activation threshold for a significant population of neurons at the target site. The present inventors also believe that certain sub-threshold simulation lowers the threshold at which neurons are activated in response to physical or cognitive input to produce a lasting change in the membrane potential such that the neurons may eventually "fire" in response to motor or cognitive functions after termination of the stimulus. The optimization procedure for sub-threshold simulation accordingly seeks to select stimulus parameters that produce the desired neural-activity at the lowest level of stimulation.

[0056] Referring to the flow diagram of Figure 7, this figure illustrates an embodiment of a method 700 including a setup procedure 710 in which the configuration of therapy electrodes and the parameters for the stimulus are selected. The therapy electrode configuration and the stimulus parameters can be determined by optimizing them as described above with reference to Figures 1-6. The method 700 then continues with an activation threshold determination procedure 720 that determines the intensity of the electrical current for the stimulus that causes a reaction in a population of the neurons at the target location to exceed the membrane activation threshold. In one embodiment, the threshold determination procedure 720 involves sensing responses in the patient that are related to changes in the membrane potential of the neurons. It is difficult to measure the actual membrane potential of a neuron, so the determination procedure 720 generally

measures a tangible response that is a surrogate for the change in the membrane potential. One such surrogate measurement of changes in the membrane potential is the EMG response to the stimulus applied to the therapy electrodes. The threshold determination procedure 720 accordingly involves adjusting the stimulus parameters until the electrical current intensity just begins to produce an EMG response indicating that a significant population of neurons at the target location have just exceeded their membrane potential. After the EMG indicates a threshold electrical current, the method 700 includes a delaying period 730 in which the effects of the supra-threshold stimulus are allowed to "wash out" from the neurons.

[0057] The method 700 further includes a sub-threshold stimulation procedure involving a selecting procedure 740 in which the intensity of the electrical current is lowered to a "sub-threshold" level, and a stimulation procedure 750 in which the sub-threshold stimulus is applied to the configuration of therapy electrodes. The selecting procedure 740 can involve selecting an electrical current that is a percentage of the threshold electrical current identified in the threshold determination procedure 720. In one embodiment, the sub-threshold current intensity is initially selected to be from approximately 40%-99% of the threshold electrical current membrane. After the sub-threshold electrical current intensity has been applied to the electrode configuration in the stimulation procedure 750, a sensing procedure 760 determines whether the sub-threshold stimulus reduced the membrane activation threshold for a population of neurons.

[0058] The sensing procedure 760 can proceed in a manner similar to the activation threshold procedure 720 explained above by applying an electrical pulse having a sensing current intensity above the sub-threshold stimulus applied in the stimulating procedure 740 and below the initial threshold stimulus level that was measured in the threshold determining procedure 720. For example, if the threshold current for the threshold stimulus that produced the threshold activation was 10 mA and the sub-threshold current applied in the stimulating procedure 750 was 7 mA, then the sensing

procedure 760 can start with a sensing current intensity of 7.5 mA and incrementally increase the sensing current intensity (e.g., by 0.5 mA increments). The sensing current is increased until the EMG measurements indicate that the membrane potential of a population of neurons has been exceeded. This is a ramp up procedure that works up from the sub-threshold current intensity applied in the stimulating procedure 750. An alternate embodiment is a ramp down procedure in which the sensing current intensity is initially set at a level near the threshold current intensity (e.g., 90-99%) and works down until a threshold activation is not detected. In either case, the sensing procedure 760 determines a secondary threshold current intensity corresponding to a change in the membrane threshold activation.

[0059] The method 700 then continues with an analyzing procedure 770 that determines whether the secondary current intensity is less than the initial threshold current intensity. If so, then the method 700 continues to identify that the stimulation is enhancing the plasticity of the neurons at stage 772, and then the method 700 either repeats procedures 740-760 with a lower sub-threshold electrical current intensity or it selects an optimized sub-threshold current intensity for use with the patient at stage 782. If the analyzing procedure 770 determines that the threshold activation of the neurons is not decreasing, then the method 700 proceeds to stage 774. In one embodiment in which a number of different electrical current intensities have reduced the activation threshold of the neurons, the method 700 continues from stage 774 to stage 782 to select the most effective sub-threshold current intensity that has been tested for use on the patient. In another embodiment in which the stimulus parameters applied to the therapy electrodes have not decreased the activation threshold, the method 700 can repeat procedures 740-770 to determine whether a different electrical current intensity can produce a lower activation threshold. In still another embodiment in which the activation threshold does not decrease after application of the stimulus, the method 700 can continue with stage

784 that involves adjusting the electrical configuration, the timing parameters of the electrical stimulation, and/or the target location of the electrodes. After stage 784, the method 700 can then proceed with repeating procedures 740-770 to determine whether the activation threshold can be lowered by applying the new stimulus parameters to the therapy electrodes in accordance with the changes that were made in stage 784.

[0060] From the foregoing, it will be appreciated that specific embodiments of the invention have been described herein for purposes of illustration, but that various modifications may be made without deviating from the spirit and scope of the invention. For example, the electrode arrays and sensing devices could be configured for use in cardiac applications to optimize implantable pacemakers or implantable defibrillators. It will be appreciated that the applications of the invention in the field of cardiology are embodiments of optimizing a peripheral stimulation treatment. Many aspects of the invention are also applicable to magnetic stimulation in addition to or in lieu of electrical stimulation. In magnetic applications, the parameters for the stimulation can be automatically set using the algorithms explained above for electrical stimulation; but, instead of selecting different configurations of a subcutaneous array of electrodes, the location and configuration of a magnetic transducer can be moved externally relative to the body. In still further applications of the inventions, many of the embodiments of the apparatus and methods can be particularly useful for optimizing spinal cord stimulation therapies and procedures. Accordingly, the invention is not limited except as by the appended claims.

CLAIMS

WHAT IS CLAIMED IS:

1. A neuro-stimulation system, comprising:

an electrode array having an implantable support member configured to be implanted into a patient and a plurality of therapy electrodes carried by the support member;

a pulse system operatively coupled to the therapy electrodes, the pulse system delivering a stimulus to the therapy electrodes; and

a controller operatively coupled to the pulse system, the controller including a computer operable medium containing instructions that generate command signals that define the stimulus delivered by the pulse system and determine a desired configuration for the therapy electrodes and/or a desired stimulus to be delivered to the therapy electrodes based upon feedback input to the controller.
2. The system of claim 1 wherein the therapy electrodes are independently coupled to the pulse system such that the pulse system can activate and/or deactivate individual therapy electrodes.
3. The system of claim 1 wherein the pulse system and the electrode array are components of an integrated unit configured to be implanted in the patient at a stimulation site.
4. The system of claim 1 wherein the electrode array is configured to be implanted at a stimulation site in the patient and the pulse system is separate

from the electrode array and configured to be implanted at a site in the patient remote from the stimulation site, and the pulse system being coupled to the electrode array by a conductive line implanted in the patient.

5. The system of claim 1 wherein the controller is configured to be external to the patient and the pulse system is configured to be implanted in the patient, and wherein the pulse system is linked to the controller via a direct link or an indirect link such that the controller can direct the pulse system to activate and/or deactivate the electrodes independently.

6. The system of claim 1, further comprising a sensing device configured to be attached to a sensing location of the patient, the sensing device generating response signals defining the feedback input into the controller; and wherein the computer operable medium contains instructions that evaluate the response signals from the sensing device.

7. The system of claim 6 wherein the sensing device comprises a sense electrode configured to be attached to the patient at a sense location to sense a response to the stimulus applied to the therapy electrodes.

8. The system of claim 6 wherein the sensing device comprises a sense electrode configured to be attached to the patient at a sense location and an EMG unit coupled to the sense electrode.

9. The system of claim 6 wherein the sensing device comprises a functional MRI device that detects locations of neural-activity in the brain.

10. The system of claim 6 wherein the computer operable medium of the controller comprises a computer readable medium containing instructions causing the controller to perform the following method:

applying an electrical stimulus having a plurality of stimulus parameters to a selected configuration of the therapy electrodes;

sensing a response to the applied electrical stimulus using the sensing device;

determining whether the response is within a desired range or an improvement over a previous sensed response from a different electrical stimulus and/or a different configuration of therapy electrodes;

selecting an alternate configuration of the therapy electrodes and/or an alternate electrical stimulus;

repeating the applying, sensing, determining and selecting procedures using the alternate configuration of the therapy electrodes and/or the alternate electrical stimulus; and

choosing a configuration of therapy electrodes and/or an electrical stimulus corresponding to a sensed response that is within a desired range and/or is an improvement compared to other sensed responses.

11. The system of claim 6 wherein the computer operable medium of the controller comprises a computer readable medium containing instructions causing the controller to perform the following method:

sending a command signal from the controller to the pulse system;

delivering an electrical pulse from the pulse system to a configuration of the therapy electrodes;

sensing a response to the electrical pulse using the sensing device;

receiving a response signal from the sensing device at the controller;

in the controller, determining whether the signal is within a desired range or an improvement over a previous response signal from another electrical pulse and/or another configuration of the therapy electrodes, and selecting an alternate configuration of the therapy electrodes and/or an alternate electrical pulse;

repeating the sending, delivering, sensing, receiving, and determining procedures using the alternate configuration of therapy electrodes and/or the alternate electrical pulse; and

in the controller, identifying an effective pulse therapy electrode configuration and/or electrical pulse; and

storing the effective therapy electrode configuration and/or electrical parameter in a memory of the controller.

12. The system of claim 6 wherein the computer operable medium of the controller comprises a computer readable medium containing instructions causing the controller to perform the following method:

installing the electrode array at a therapy site of a patient;

installing the sensing device at a sense location of the patient;

selecting a setup configuration of the therapy electrodes and a control stimulus of electrical parameters;

applying the control stimulus to the therapy electrodes;

sensing a response in the patient with the sensing device and generating a response signal;

in the controller, evaluating the response signal by comparing the response signal with at least one of a desired response signal and/or an antecedent response signal sensed by the sensing device that have been stored in a memory of the controller;

in the controller, automatically choosing an alternate configuration of therapy electrodes according to the evaluation of the response signal with the desired response signal and/or the antecedent response signal;

reapplying the control stimulus to the alternate configuration of therapy electrodes and sensing a response signal using the sensing device;
and

repeating the evaluating, choosing and reapplying procedures until the response signal is within a desired range and/or a desired number of therapy electrode configurations have been tested.

13. The system of claim 6 wherein the computer operable medium of the controller comprises a computer readable medium containing instructions causing the controller to perform the following method:

installing the electrode array at a therapy site of a patient;

installing the sensing device at a sense location of the patient;

applying an electrical stimulus having a plurality of stimulus parameters to a control configuration of therapy electrodes;

sensing a response in the patient with the sensing device and generating a response signal;

in the controller, evaluating the response signal by comparing the response signal with at least one of a desired response signal and/or an

antecedent response signal sensed by the sensing device stored in a memory of the controller;

in the controller, automatically choosing an alternate set of stimulus parameters according to the evaluation of the response signal with the desired response signal and/or the antecedent response signal;

reapplying the alternate set of stimulus parameters to the setup configuration of therapy electrodes and sensing a response signal using the sensing device; and

repeating the evaluating, choosing and reapplying procedures until the response signal is within a desired range and/or a desired number of stimulus parameters have been tested.

14. The system of claim 6 wherein the computer operable medium of the controller comprises a computer readable medium containing instructions causing the controller to perform the following method:

selecting an initial set of stimulation parameters for an initial electrical stimulus;

applying the initial electrical stimulus to a configuration of the therapy electrodes at a target stimulation site of the patient;

sensing a response signal at a sensing site of the patient that corresponds to the initial electrical stimulus applied to the therapy electrodes;

independently adjusting a current intensity until a threshold electrical stimulus is identified, the threshold electrical stimulus having a threshold current intensity at which a response is first identified in a population of neurons of the target site; and

applying a sub-threshold electrical stimulus to the configuration of therapy electrodes, the sub-threshold electrical stimulus having a current intensity less than the current intensity of the threshold electrical stimulus.

15. In a computer, a method of automatically determining a favorable neuro-stimulation program for a patient, comprising:

applying an electrical stimulus having a plurality of stimulus parameters to a selected configuration of the therapy electrodes that have been installed at a target therapy site of a patient;

sensing a response to the applied electrical stimulus at a sensing device that has been installed at a sense location of the patient;

determining whether the response is within a desired range or an improvement over a previous sensed response from a different electrical stimulus and/or a different configuration of therapy electrodes;

selecting an alternate configuration of therapy electrodes and/or an alternate electrical stimulus;

repeating the applying, sensing, determining and selecting procedures using the alternate configuration of therapy electrodes and/or the alternate electrical stimulus; and

choosing a configuration of therapy electrodes and/or an electrical stimulus corresponding to a sensed response that is within a desired range and/or provides a better result compared to other sensed responses.

16. The method of claim 15 wherein the selecting procedure comprises computing an alternate stimulus parameter while maintaining a constant electrode

configuration, and wherein computing the alternate stimulus parameter comprises correlating a plurality of different stimuli applied to the constant electrode configuration with corresponding sensed responses to determine a stimulus/response trend and estimating a new stimulus parameter that is expected to improve the efficacy according to the stimulus/response trend.

17. The method of claim 15 wherein the selecting procedure comprises computing an alternate electrode configuration while maintaining constant stimulus parameters, and wherein computing the alternate electrode configuration comprises correlating a plurality of sensed responses with corresponding electrode configurations to which the constant stimulus parameters were applied to determine an electrode-configuration/response trend and estimating a new electrode configuration that is expected to improve the efficacy according to the electrode-configuration/response trend.

18. The method of claim 15 wherein the selecting procedure comprises increasing a stimulus parameter when a stimulus/response trend indicates that an increase in the stimulus parameter improves the efficacy of the stimulus.

19. The method of claim 15 wherein the selecting procedure comprises decreasing a stimulus parameter when a stimulus/response trend indicates that a decrease in the stimulus parameter improves the efficacy of the stimulus.

20. The method of claim 15 wherein the applying, sensing, determining, selecting, repeating and choosing procedures are repeated on the same patient within a period not greater than one week.

21. The method of claim 15 wherein the applying, sensing, determining, selecting, repeating and choosing procedures are repeated on the same patient on consecutive days.

22. The method of claim 15 wherein the applying, sensing, determining and selecting procedures are completed in a time period not greater than approximately 300 seconds.

23. The method of claim 15 wherein two iterations of the applying, sensing, determining and selecting procedures are repeated in a time period not greater than approximately 90 seconds.

24. The method of claim 15 wherein two iterations of the applying, sensing, determining and selecting procedures are repeated in a time period not greater than approximately 180 seconds.

25. The method of claim 15 wherein two iterations of the applying, sensing, determining and selecting procedures are repeated in a time period of approximately 20-90 seconds.

26. The method of claim 15 wherein a single iteration of the applying, sensing, determining and selecting procedures is completed in a time period not greater than approximately 45 seconds.

27. The method of claim 15 wherein a single iteration of the applying, sensing, determining and selecting procedures is completed in a time period of approximately 10-30 seconds.

28. The method of claim 15 wherein the sensing procedure comprises attaching EMG sensors to a sense site of the patient, detecting peripheral responses to the stimuli applied to the electrodes, and automatically sending the detected peripheral responses to the controller.

29. The method of claim 15 wherein the sensing procedure comprises detecting data related to neural activity using a functional MRI and automatically sending the data to the controller.

30. The method of claim 15 wherein the data comprises coordinates of neural activity relative to the therapy electrodes.

31. The method of claim 15 wherein the data comprises intensity levels of neural activity.

32. In a computer, a method of automatically determining a favorable a neuro-stimulation program for a patient, comprising:

 sending a command signal from a controller to a pulse system operatively coupled to the controller;

 delivering an electrical pulse from the pulse system to a configuration of therapy electrodes in a therapy electrode array installed at a target stimulation site of a patient;

 sensing a response to the electrical pulse at a sensing device installed at a sense location of the patient;

 receiving a response signal from the sensing device at the controller;

 in the controller, determining whether the signal is within a desired range or an improvement over a previous response signal from another electrical pulse and/or another configuration of therapy electrodes, and selecting an alternate configuration of therapy electrodes and/or an alternate electrical pulse;

repeating the sending, delivering, sensing, receiving, and determining procedures using the alternate configuration of therapy electrodes and/or the alternate electrical pulse; and

in the controller, identifying an effective pulse therapy electrode configuration and/or electrical pulse; and

storing the effective therapy electrode configuration and/or electrical pulse in a memory of the controller.

33. The method of claim 32 wherein the selecting procedure comprises computing an alternate stimulus parameter while maintaining a constant electrode configuration, and wherein computing the alternate stimulus parameter comprises correlating a plurality of different stimuli applied to the constant electrode configuration with corresponding sensed responses to determine a stimulus/response trend and estimating a new stimulus parameter that is expected to improve the efficacy according to the stimulus/response trend.

34. The method of claim 32 wherein the selecting procedure comprises computing an alternate electrode configuration while maintaining constant stimulus parameters, and wherein computing the alternate electrode configuration comprises correlating a plurality of sensed responses with corresponding electrode configurations to which the constant stimulus parameters were applied to determine an electrode-configuration/response trend and estimating a new electrode configuration that is expected to improve the efficacy according to the electrode-configuration/response trend.

35. The method of claim 32 wherein the selecting procedure comprises increasing a stimulus parameter when a stimulus/response trend indicates that an increase in the stimulus parameter improves the efficacy of the stimulus.

36. The method of claim 32 wherein the selecting procedure comprises decreasing a stimulus parameter when a stimulus/response trend indicates that a decrease in the stimulus parameter improves the efficacy of the stimulus.

37. The method of claim 32 wherein two iterations of the applying, sensing, determining and selecting procedures are repeated in a time period not greater than approximately 90 seconds.

38. The method of claim 32 wherein two iterations of the applying, sensing, determining and selecting procedures are completed in a time period not greater than approximately 180 seconds.

39. The method of claim 32 wherein the sensing procedure comprises attaching EMG sensors to a sense site of the patient, detecting peripheral responses to the stimuli applied to the electrodes, and automatically sending the detected peripheral responses to the controller.

40. The method of claim 32 wherein the sensing procedure comprises detecting data related to neural activity using a functional MRI and automatically sending the data to the controller.

41. A method of automatically determining a favorable neuro-stimulation program for a patient, comprising:

installing an electrode array having a plurality of therapy electrodes at a therapy site of a patient;

installing a sensing device at a sense location of the patient;

selecting a setup configuration of therapy electrodes and a control stimulus of electrical parameters;

applying the control stimulus to the therapy electrodes;

sensing a response in the patient with the sensing device and generating a response signal;

in the controller, evaluating the response signal by comparing the response signal with at least one of a desired response signal and/or an antecedent response signal sensed by the sensing device that have been stored in a memory of the controller;

in the controller, automatically choosing an alternate configuration of therapy electrodes according to the evaluation of the response signal with the desired response signal and/or the antecedent response signal;

reapplying the control stimulus to the alternate configuration of therapy electrodes and sensing a response signal using the sensing device;
and

repeating the evaluating, choosing and reapplying procedures until the response signal is within a desired range and/or a desired number of therapy electrode configurations have been tested.

42. A method of automatically determining a favorable neuro-stimulation program for a patient, comprising:

installing an electrode array having a plurality of therapy electrodes at a therapy site of a patient;

installing a sensing device at a sense location of the patient;

applying an electrical stimulus having a plurality of stimulus parameters to a control configuration of therapy electrodes;

sensing a response in the patient with the sensing device and generating a response signal;

in the controller, evaluating the response signal by comparing the response signal with at least one of a desired response signal and/or an antecedent response signal sensed by the sensing device stored in a memory of the controller;

in the controller, adjusting at least one of the stimulus parameters according to the evaluation of the response signal with the desired response signal and/or the antecedent response signal;

reapplying the adjusted stimulus parameters to the setup configuration of therapy electrodes and sensing a response signal using the sensing device; and

repeating the evaluating, choosing and reapplying procedures until the response signal is within a desired range and/or a desired number of stimulus parameters have been tested.

43. A method of automatically determining a favorable sub-threshold neuro-stimulation program for a patient, comprising:

selecting a set of stimulation parameters for an electrical stimulus;

applying the electrical stimulus to a configuration of therapy electrodes at a target stimulation site of the patient;

sensing a response signal at a sensing site of the patient that corresponds to the electrical stimulus applied to the therapy electrodes;

independently adjusting a current intensity until a threshold electrical stimulus is identified, the threshold electrical stimulus having a

threshold current intensity at which a response is first identified in a population of neurons of the target site; and

applying a sub-threshold electrical stimulus to the configuration of therapy electrodes, the sub-threshold electrical stimulus having a current intensity less than the current intensity of the threshold electrical stimulus.

44. The method of claim 43 wherein applying a sub-threshold stimulus comprises applying a sub-threshold current intensity of approximately 40-99% of the threshold current intensity.

45. The method of claim 43 wherein applying a sub-threshold stimulus comprises applying a sub-threshold current intensity of approximately 60-80% of the threshold current intensity.

46. The method of claim 43 wherein applying a sub-threshold stimulus comprises applying a sub-threshold current intensity of approximately 68-72% of the threshold current intensity.

47. The method of claim 43 wherein:

applying a sub-threshold stimulus comprises applying a sub-threshold current intensity of approximately 40-99% of the threshold current intensity; and

the method further comprises determining whether the application of the sub-threshold current intensity decreased a membrane activation threshold for a population of neurons subject to the sub-threshold stimulus.

48. The method of claim 43, further comprising decreasing the sub-threshold current intensity to a lower level and re-applying the decreased sub-threshold stimulus with the lower current intensity to the neurons, and further determining whether the application of the decreased sub-threshold current intensity further decreased the membrane activation threshold for the population of neurons.

49. The method of claim 43, further comprising repeating (a) decreasing the sub-threshold current intensity to a lower level, (b) re-applying the decreased sub-threshold stimulus with the lower current intensity to the neurons, and (c) further determining whether the application of the decreased sub-threshold current intensity further decreased the membrane activation threshold for the population of neurons until the membrane activation threshold does not decreased by a desired amount.

1/12

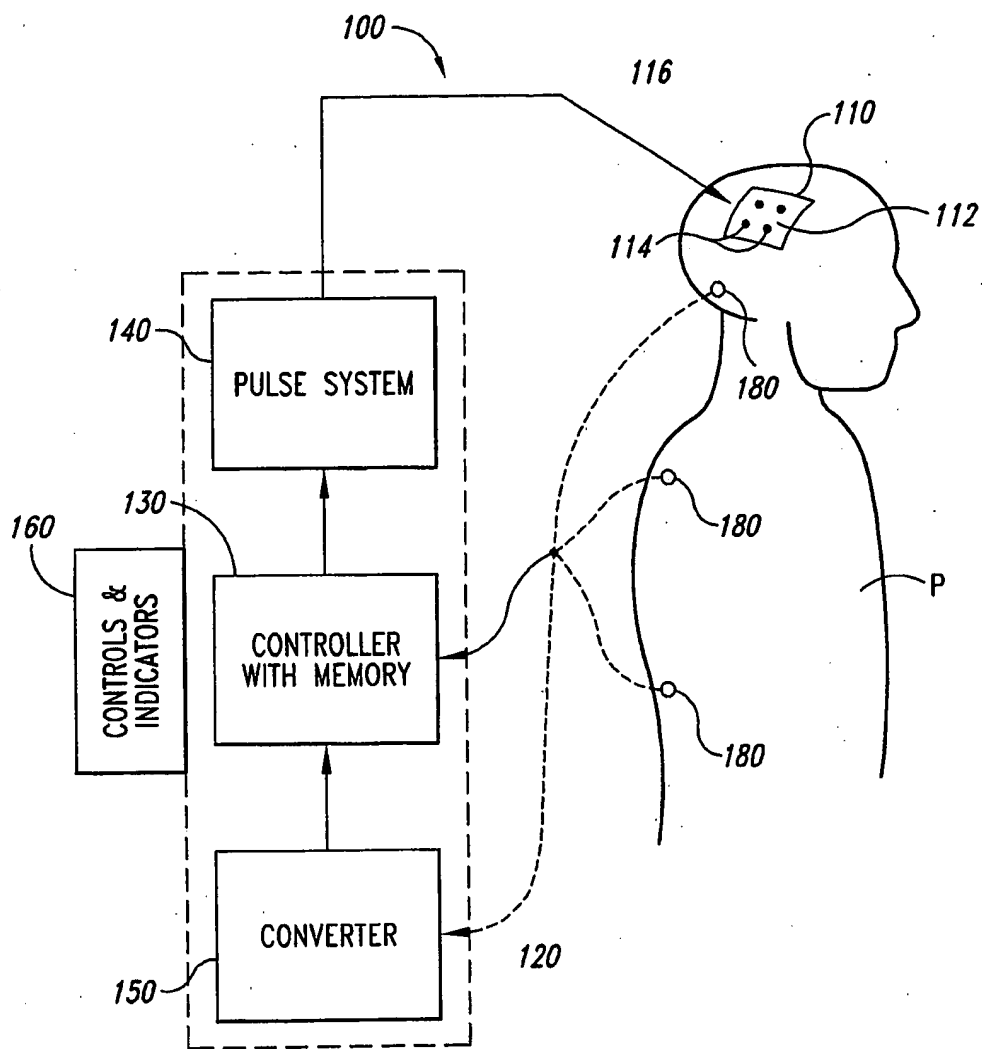
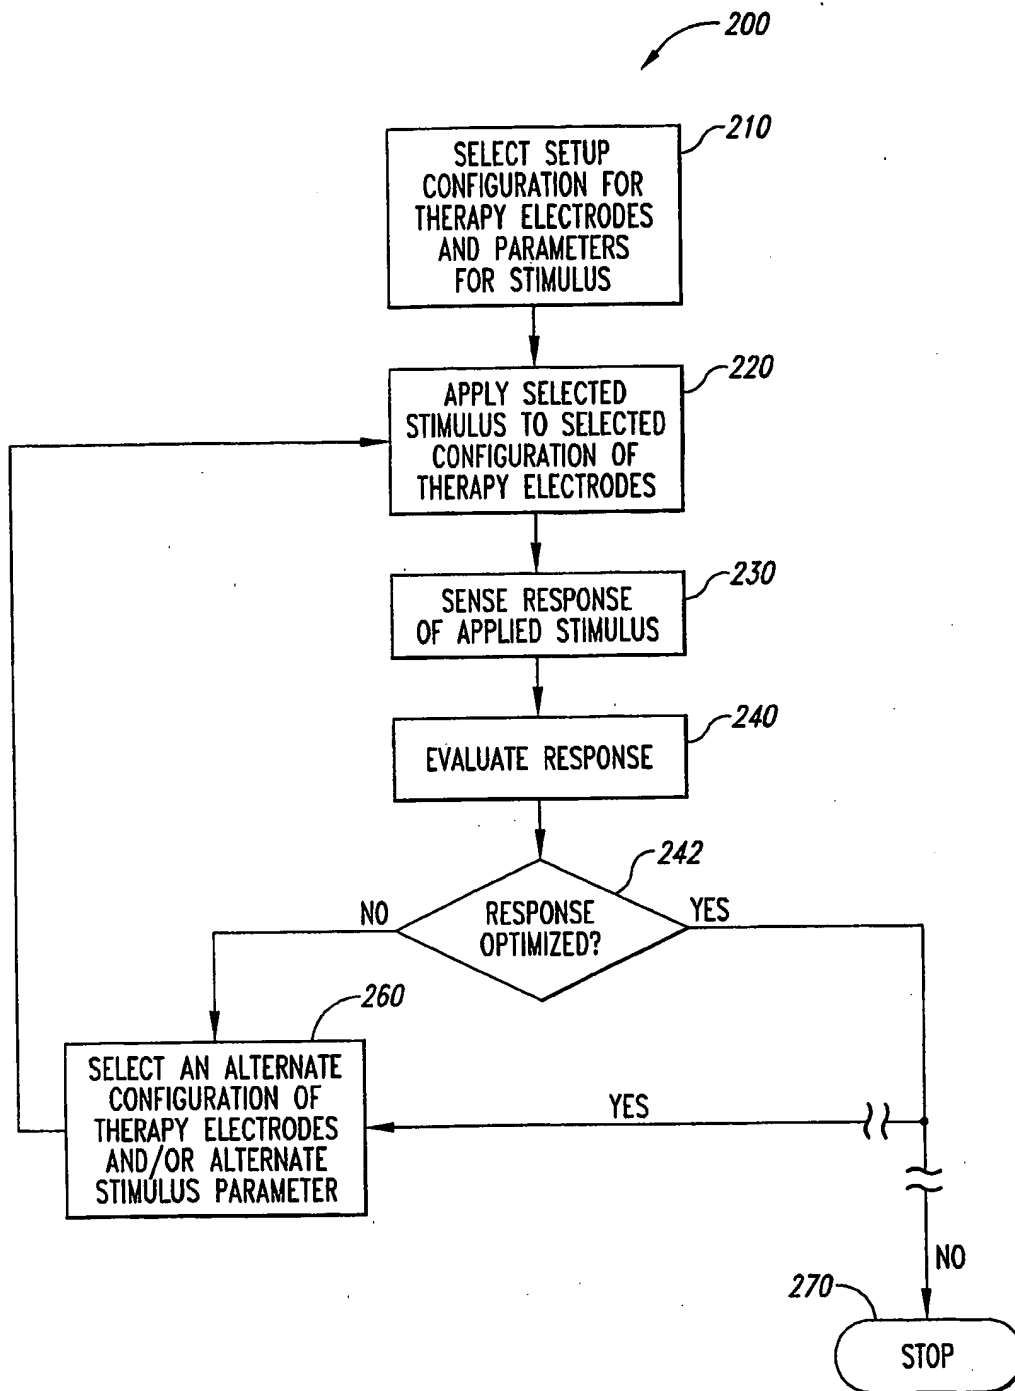
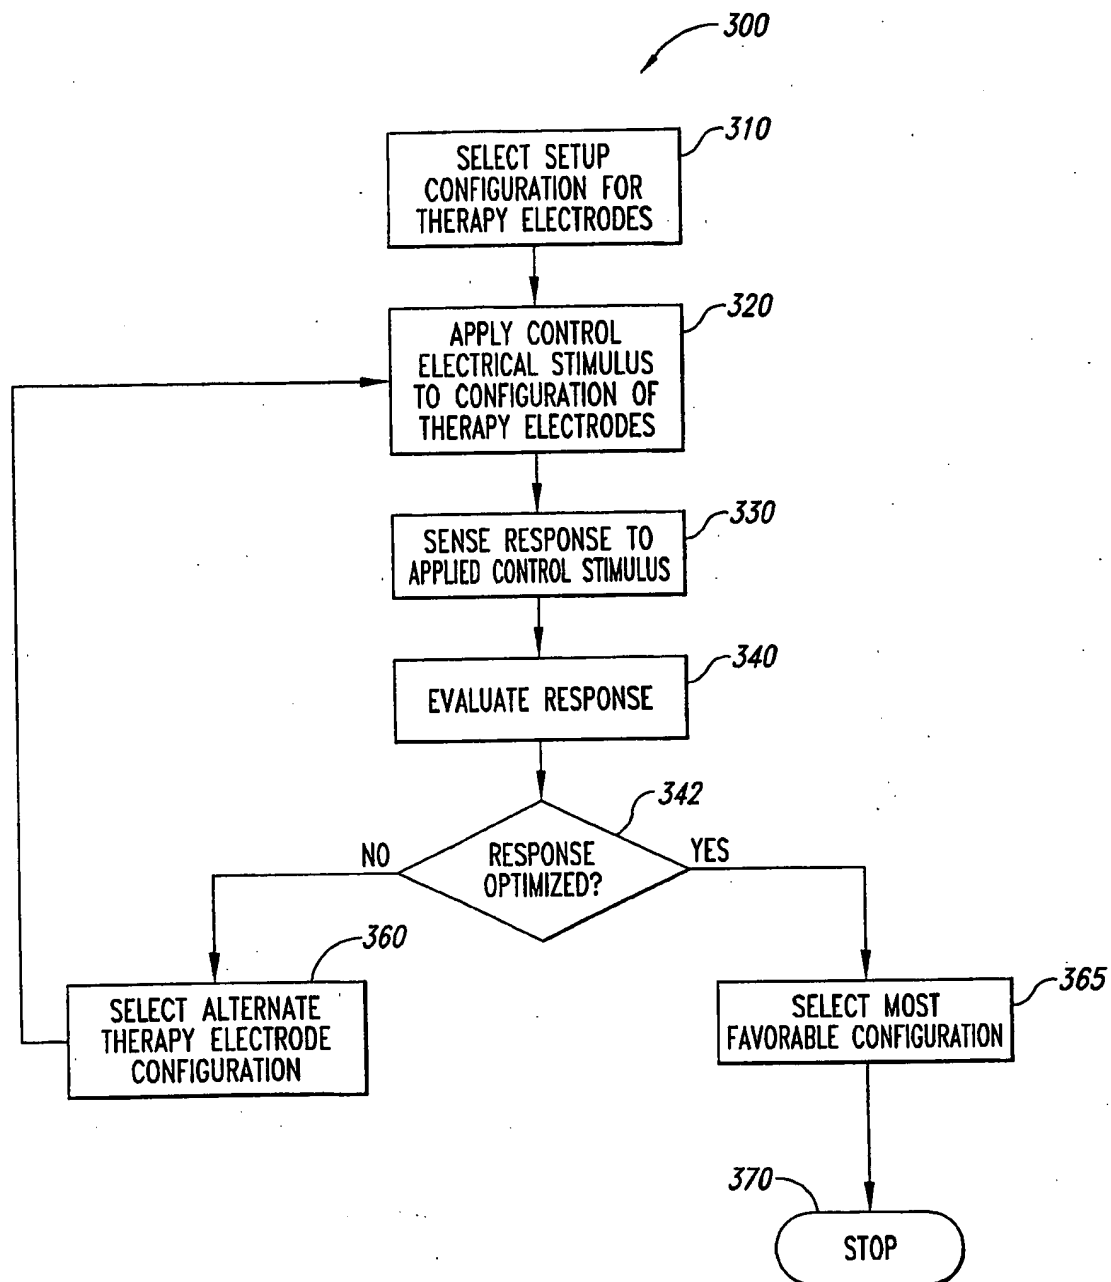


Fig. 1

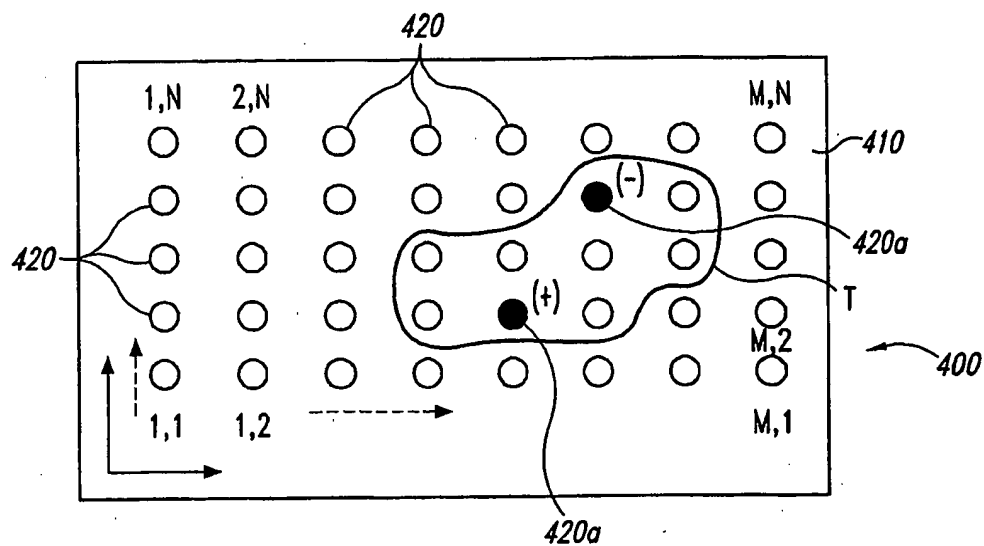
2/12

*Fig. 2*

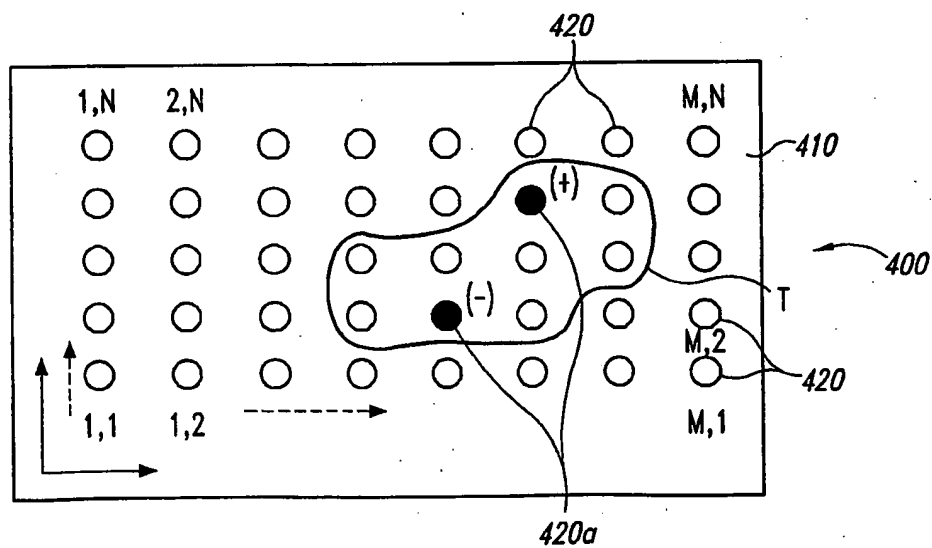
3/12

*Fig. 3*

4/12


*Fig. 4A*

○ INACTIVE ELECTRODE
● ACTIVE ELECTRODE (+ OR -)

*Fig. 4B*


○ INACTIVE ELECTRODE
● ACTIVE ELECTRODE (+ OR -)

5/12

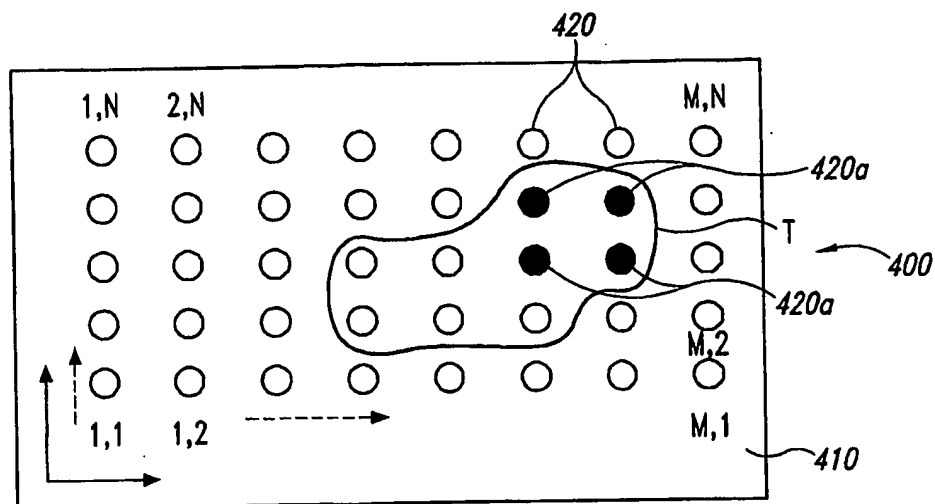

○ INACTIVE ELECTRODE
● ACTIVE ELECTRODE (+ OR -)


Fig. 4C

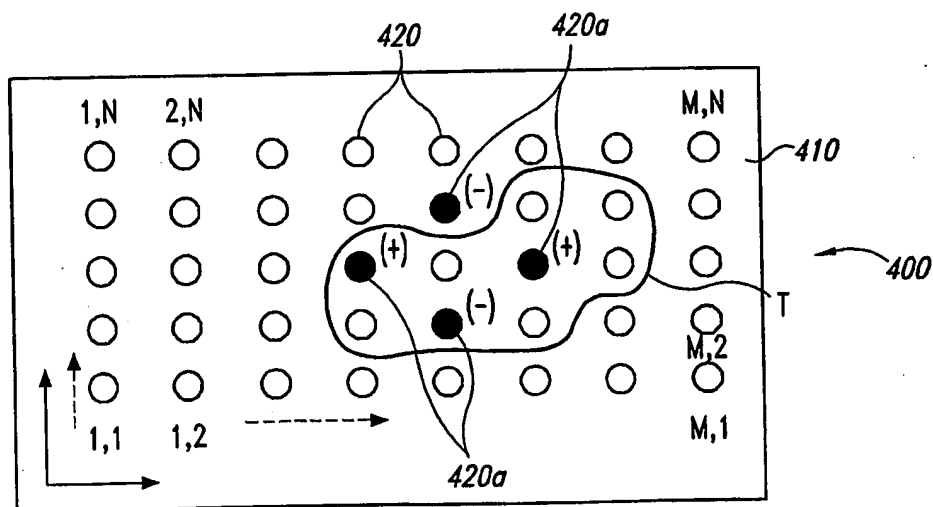


○ INACTIVE ELECTRODE
● ACTIVE ELECTRODE (+ OR -)

Fig. 4D

6/12

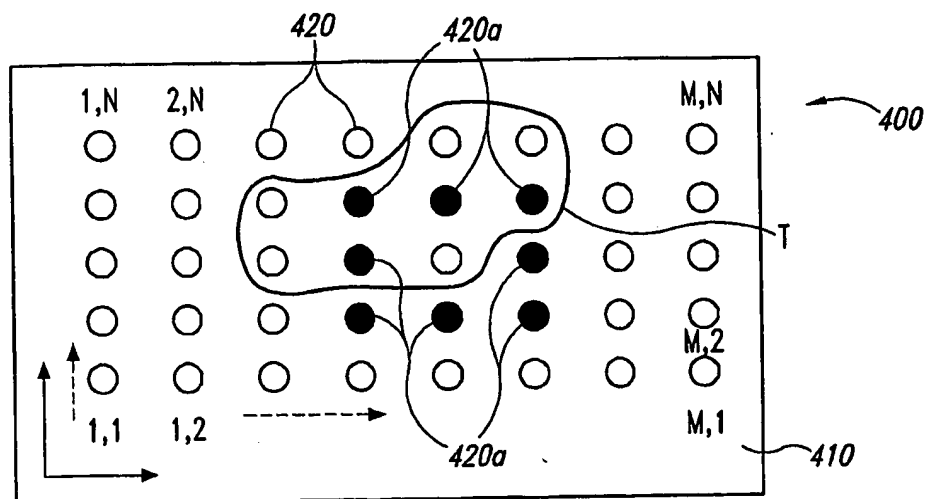*Fig. 4E*

○ INACTIVE ELECTRODE
● ACTIVE ELECTRODE (+ OR -)

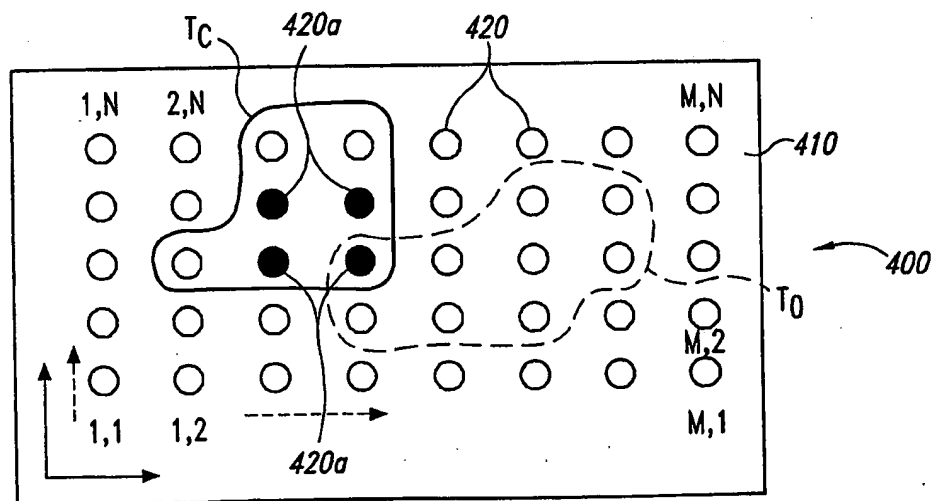*Fig. 4F*

○ INACTIVE ELECTRODE
● ACTIVE ELECTRODE (+ OR -)

7/12

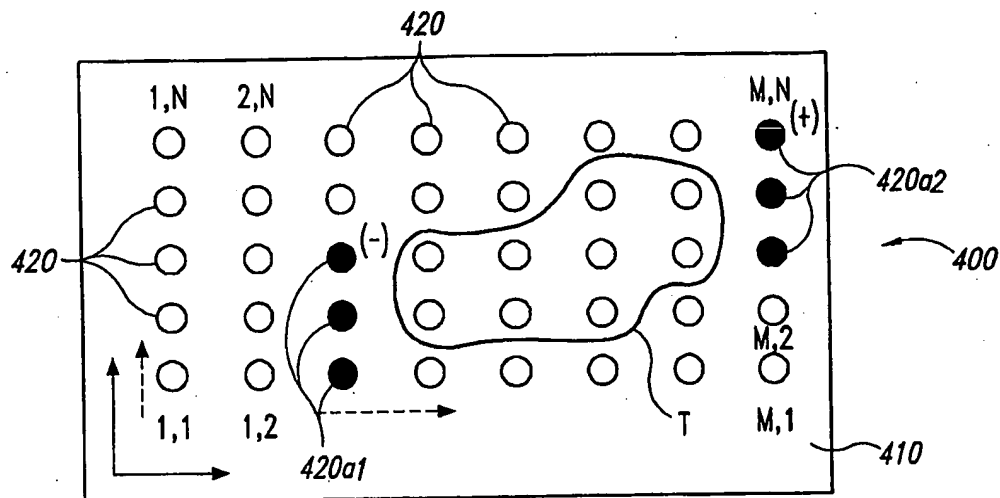


Fig. 4G


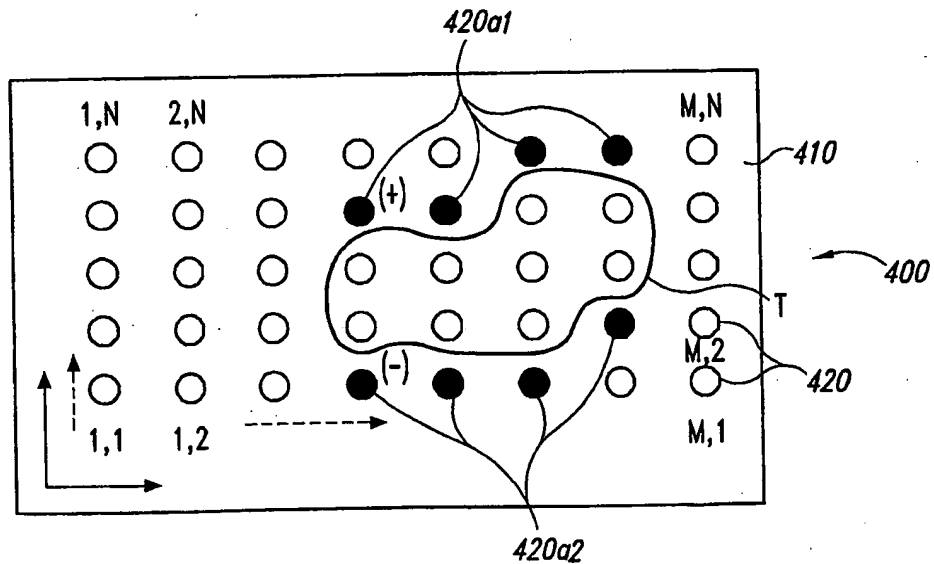



Fig. 4H

8/12

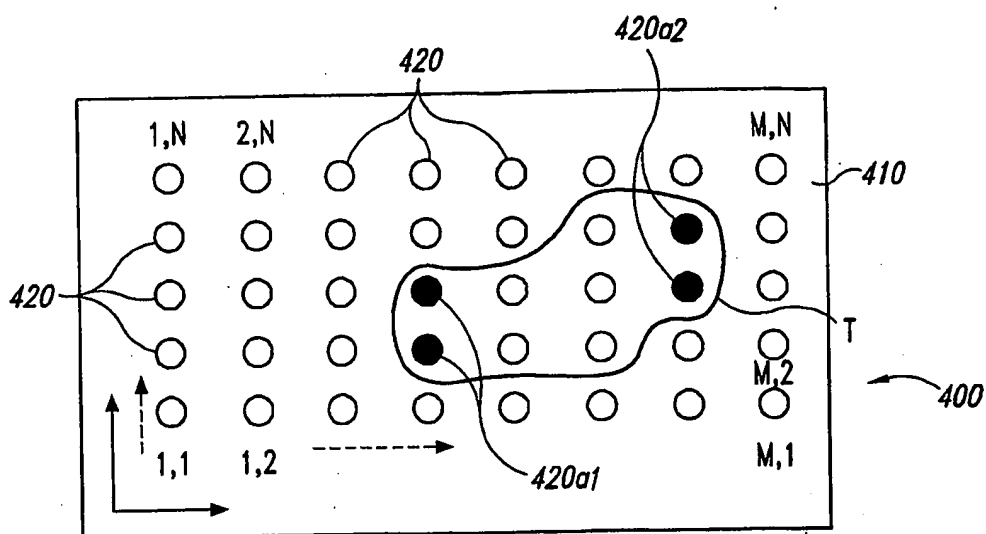

○ INACTIVE ELECTRODE
 ● ACTIVE ELECTRODE (+ OR -)

Fig. 4I

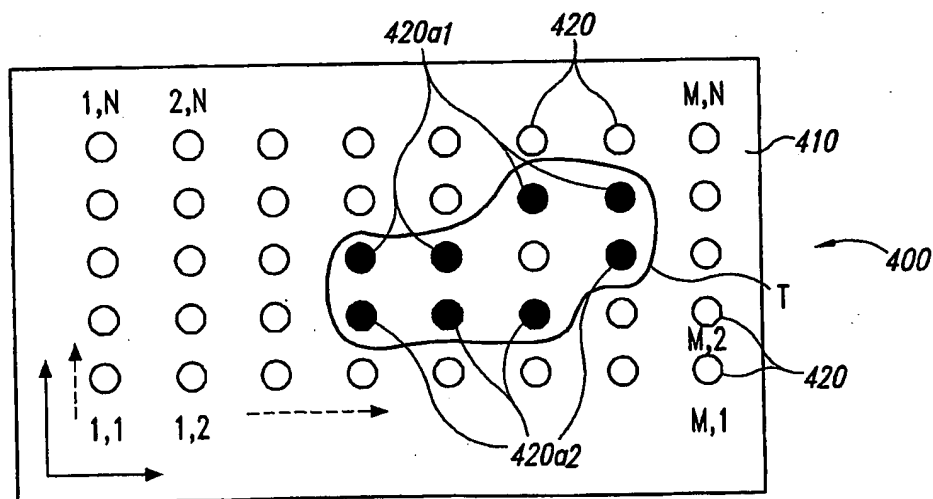

○ INACTIVE ELECTRODE
 ● ACTIVE ELECTRODE (+ OR -)

Fig. 4J

9/12

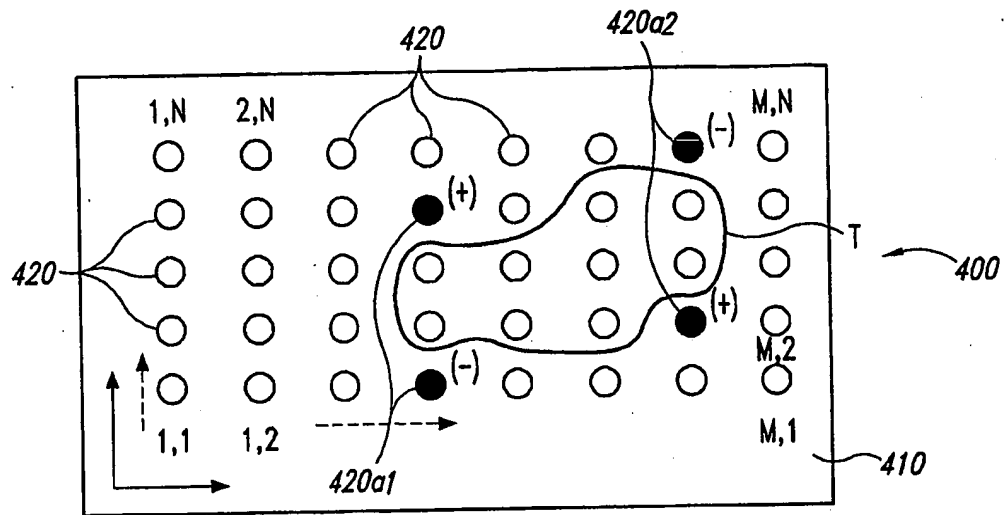


Fig. 4K

○ INACTIVE ELECTRODE
● ACTIVE ELECTRODE (+ OR -)


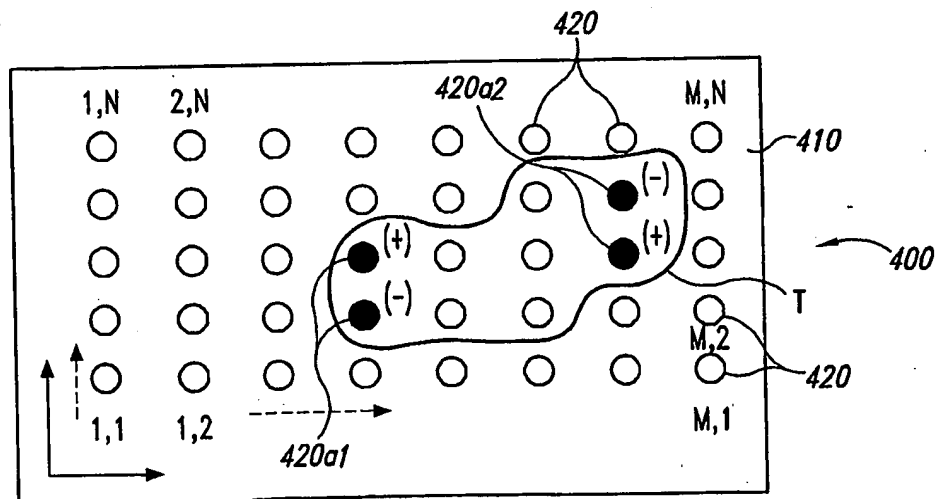


Fig. 4L

○ INACTIVE ELECTRODE
● ACTIVE ELECTRODE (+ OR -)

10/12

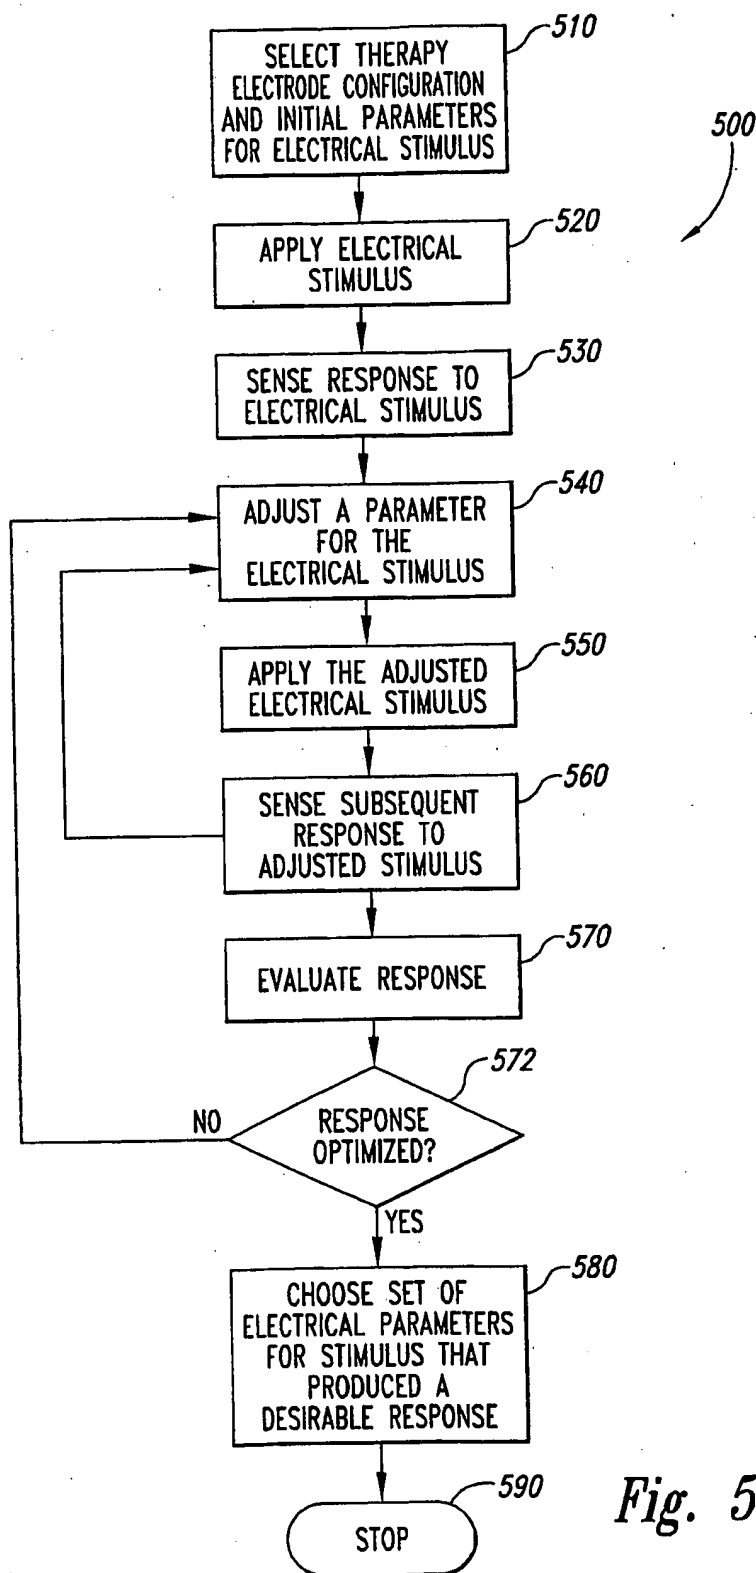

11/12

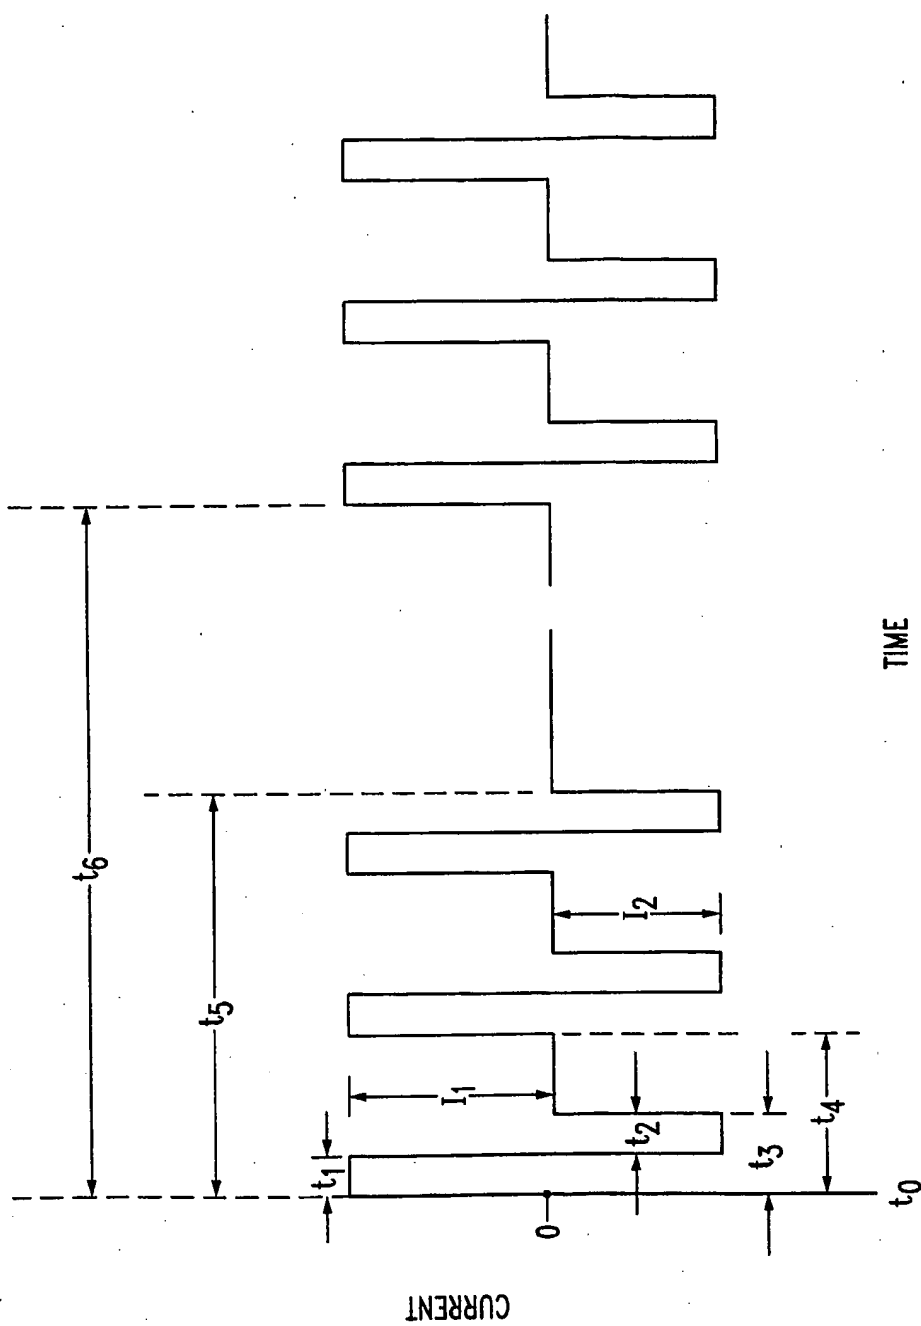


Fig. 6

12/12

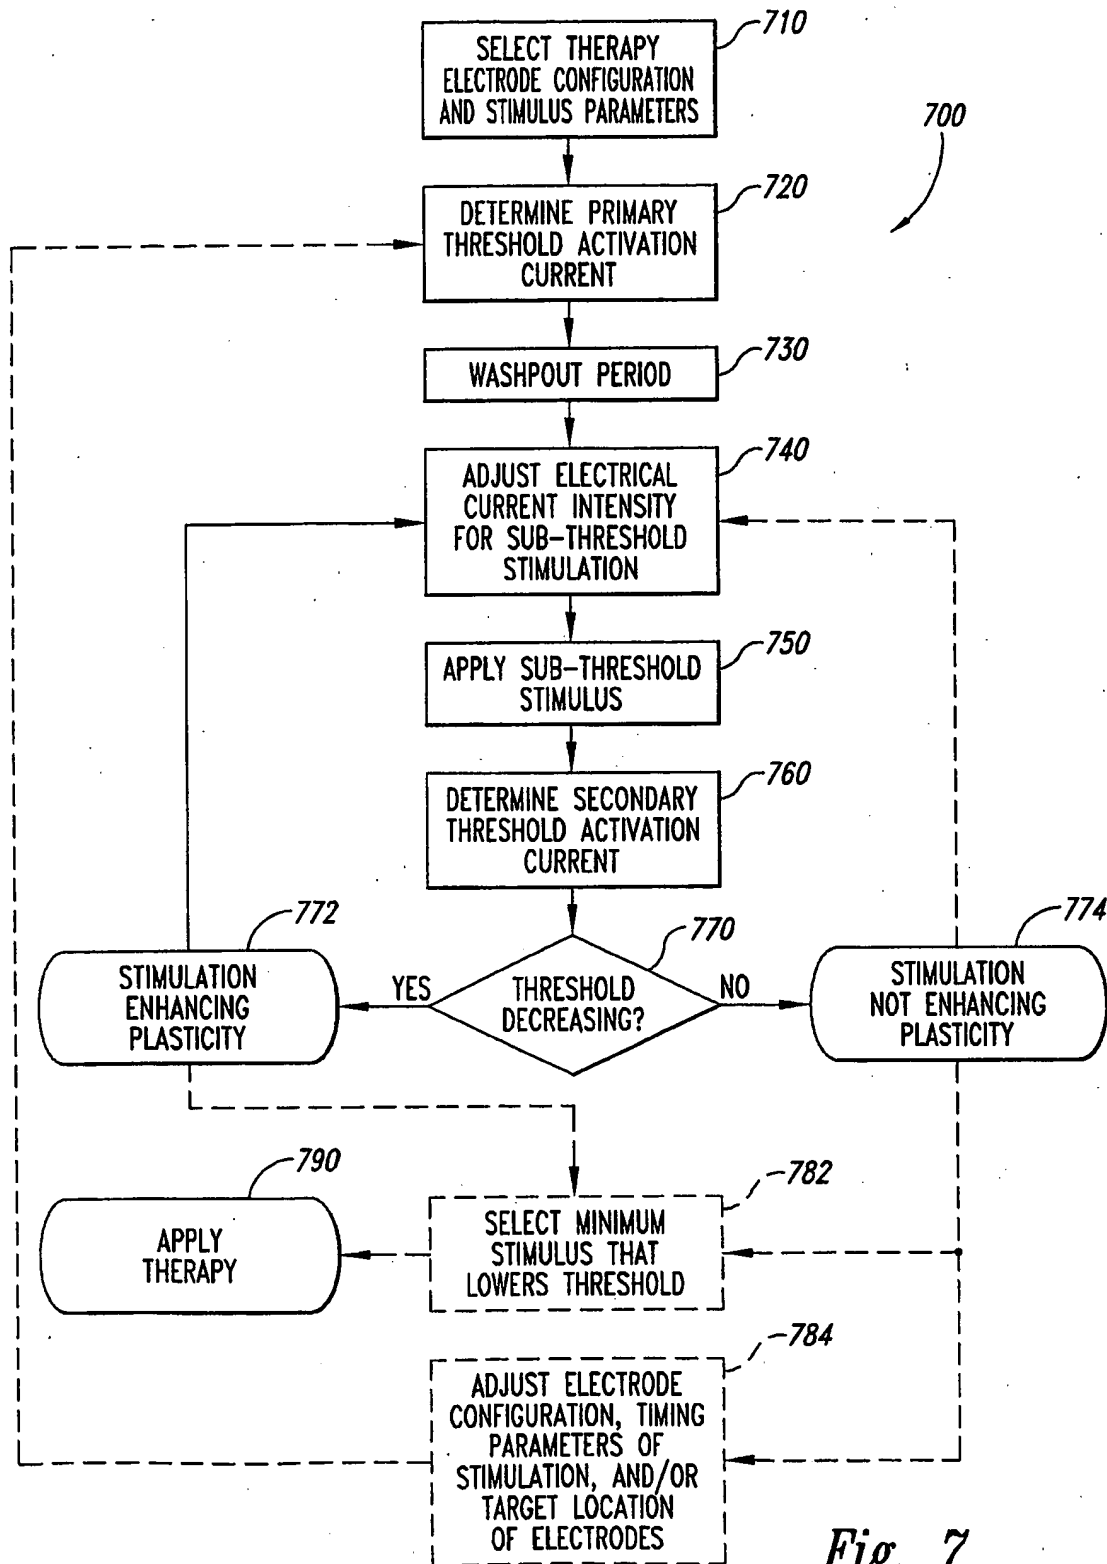


Fig. 7

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 02/32695

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61N1/36

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the International search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 6 061 593 A (UPTON ADRIAN R M ET AL) 9 May 2000 (2000-05-09) the whole document ---	1-7
X	US 5 370 672 A (FOWLER KIM R ET AL) 6 December 1994 (1994-12-06) the whole document ---	1-5
X	US 6 052 624 A (MANN CARLA M) 18 April 2000 (2000-04-18) the whole document ---	1-5
X	WO 87 07511 A (ZION EDUCATIONAL FOUND) 17 December 1987 (1987-12-17) the whole document --- -/--	1-5

☒ Further documents are listed in the continuation of box C.☒ Patent family members are listed in annex.

* Special categories of cited documents:

A document defining the general state of the art which is not considered to be of particular relevance

E earlier document but published on or after the international filing date

L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

O document referring to an oral disclosure, use, exhibition or other means

P document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

Z document member of the same patent family

Date of the actual completion of the international search

17 December 2002

Date of mailing of the international search report

27/12/2002

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Ferrigno, A

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 02/32695

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	<p>US 5 983 140 A (IGNATOSKI MICHAEL ET AL) 9 November 1999 (1999-11-09) the whole document</p> <p>-----</p>	1-5

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

Continuation of Box I.2

Claims Nos.: 12,13

Although claims 12 and 13 are apparatus claims they features relate to a method of using the apparatus, the method including the steps of implanting the apparatus.

The applicant's attention is drawn to the fact that claims, or parts of claims, relating to inventions in respect of which no international search report has been established need not be the subject of an international preliminary examination (Rule 66.1(e) PCT). The applicant is advised that the EPO policy when acting as an International Preliminary Examining Authority is normally not to carry out a preliminary examination on matter which has not been searched. This is the case irrespective of whether or not the claims are amended following receipt of the search report or during any Chapter II procedure.

INTERNATIONAL SEARCH REPORT

.....national application No.
PCT/US 02/32695

Box I Observations where certain claims were found unsearchable (Continuation of Item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 12, 13, 15-49
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery and therapy
2. ☒ Claims Nos.: 12, 13
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
see FURTHER INFORMATION sheet PCT/ISA/210
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of Item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 02/32695

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 6061593	A	09-05-2000	US 6016449 A	18-01-2000
			EP 0911061 A2	28-04-1999
			US 2002099412 A1	25-07-2002
			US 6128538 A	03-10-2000
			US 6134474 A	17-10-2000
			US 6427086 B1	30-07-2002
			US 6354299 B1	12-03-2002
			US 6360122 B1	19-03-2002
			US 2001056290 A1	27-12-2001
			US 2002002390 A1	03-01-2002
			US 2001051819 A1	13-12-2001
US 5370672	A	06-12-1994	NONE	
US 6052624	A	18-04-2000	US 6393325 B1	21-05-2002
WO 8707511	A	17-12-1987	AU 601203 B2	06-09-1990
			AU 7708987 A	11-01-1988
			BR 8707351 A	13-09-1988
			CA 1310069 A1	10-11-1992
			DK 76088 A	14-04-1988
			EP 0272318 A1	29-06-1988
			FI 880696 A	15-02-1988
			MC 1859 A	19-12-1988
			NO 880656 A	15-04-1988
			WO 8707511 A2	17-12-1987
US 5983140	A	09-11-1999	US 5861017 A	19-01-1999
			US 6424868 B1	23-07-2002
			EP 1017448 A1	12-07-2000
			JP 2002510224 T	02-04-2002
			WO 9855177 A1	10-12-1998

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☐ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.